




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022124\
Data File : BM044239.D
Acq On : 22 Feb 2024 14:30
Operator : MA/JU
Sample : P1494-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3Y4

Manual IntegrationsAPPROVED

Quant Time: Feb 22 15:07:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/22/2024
Supervised By :mohammad ahmed 02/23/2024

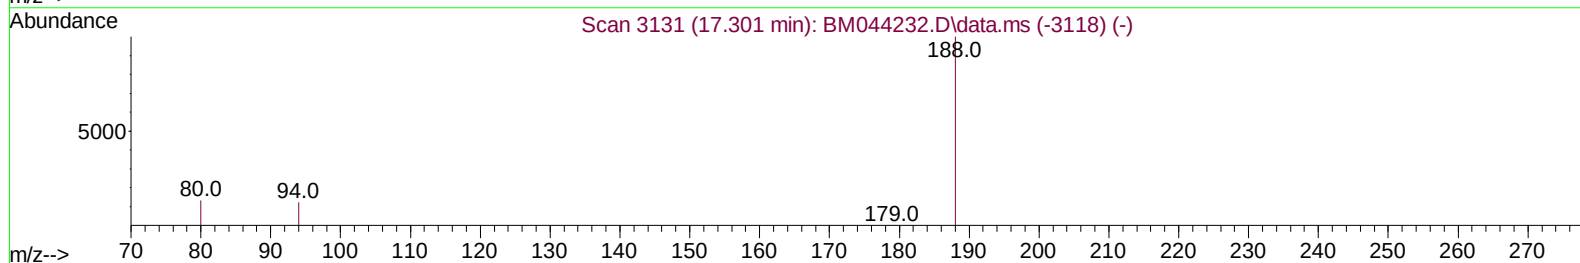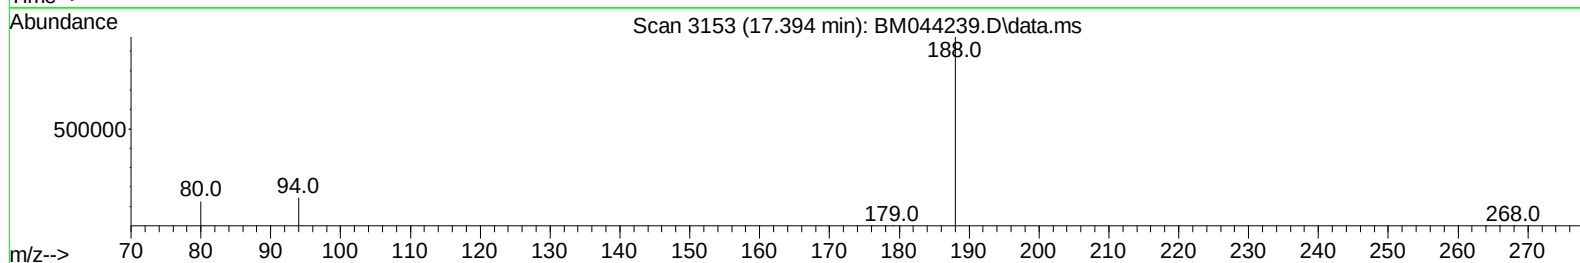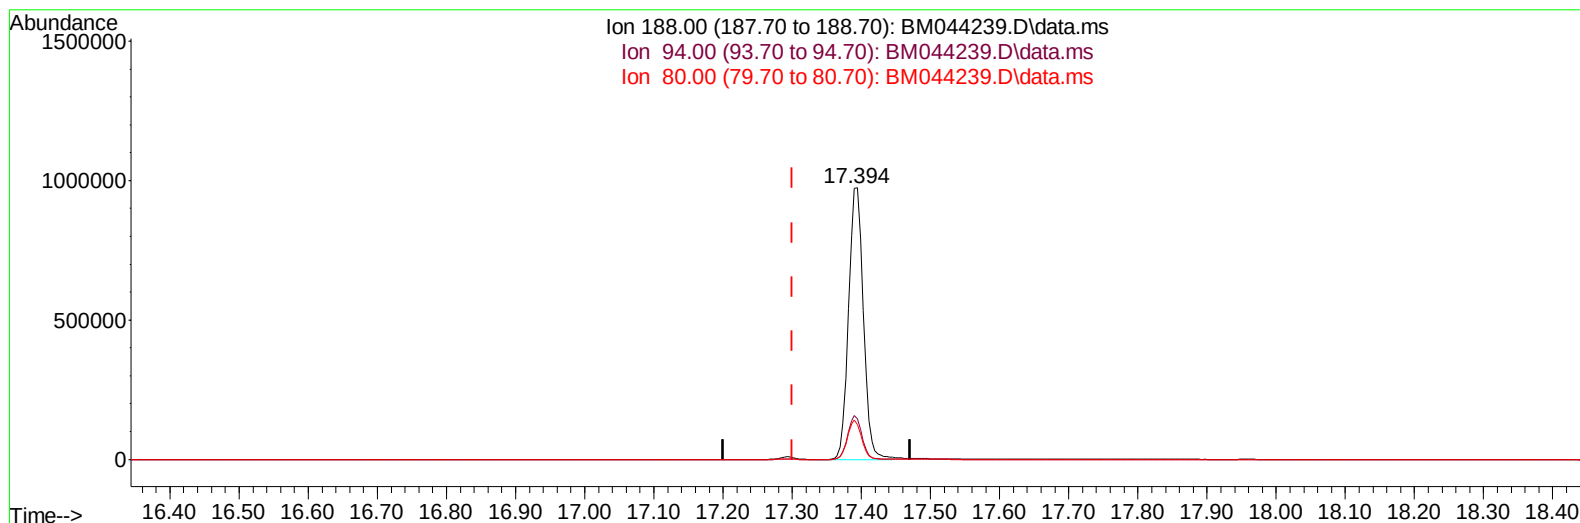

TIC: BM044239.D\data.ms

(13) Phenanthrene-d10 (I)

17.394min (+ 0.094) 0.40 ng/u1

response 1442891

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.40	14.93#
80.00	13.40	12.92
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022124\
Data File : BM044239.D
Acq On : 22 Feb 2024 14:30
Operator : MA/JU
Sample : P1494-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3Y4

Manual IntegrationsAPPROVED

Quant Time: Feb 22 15:07:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/22/2024
Supervised By :mohammad ahmed 02/23/2024

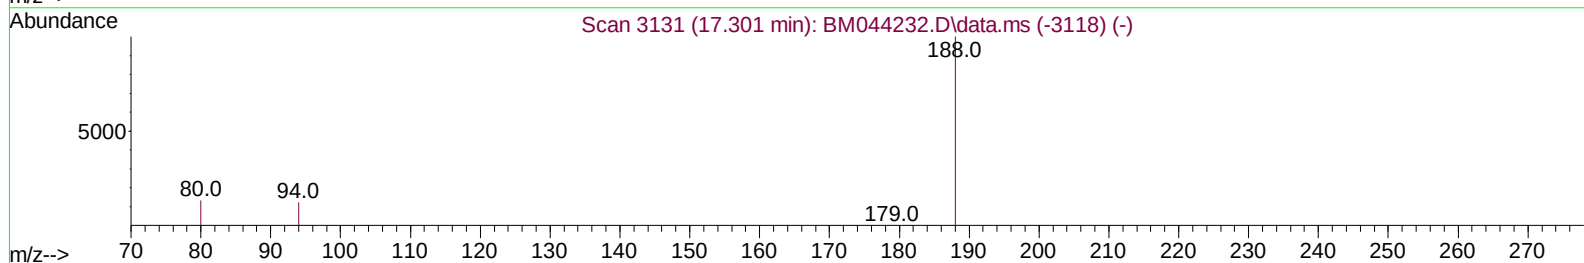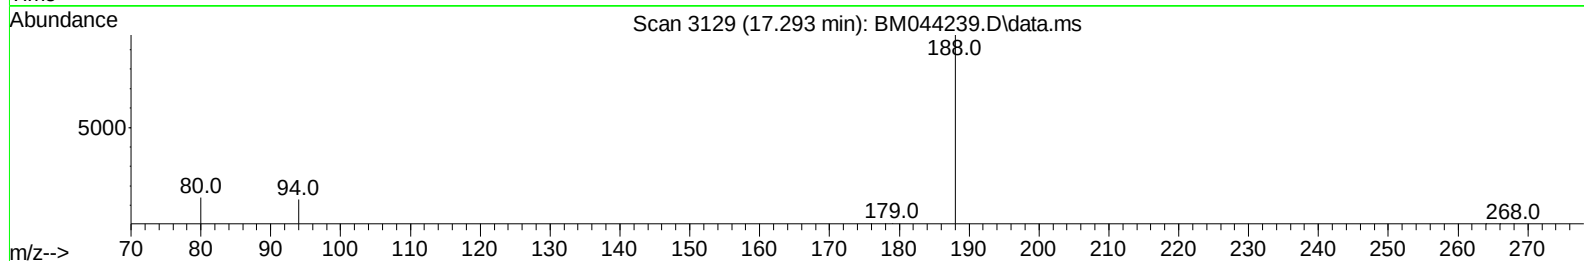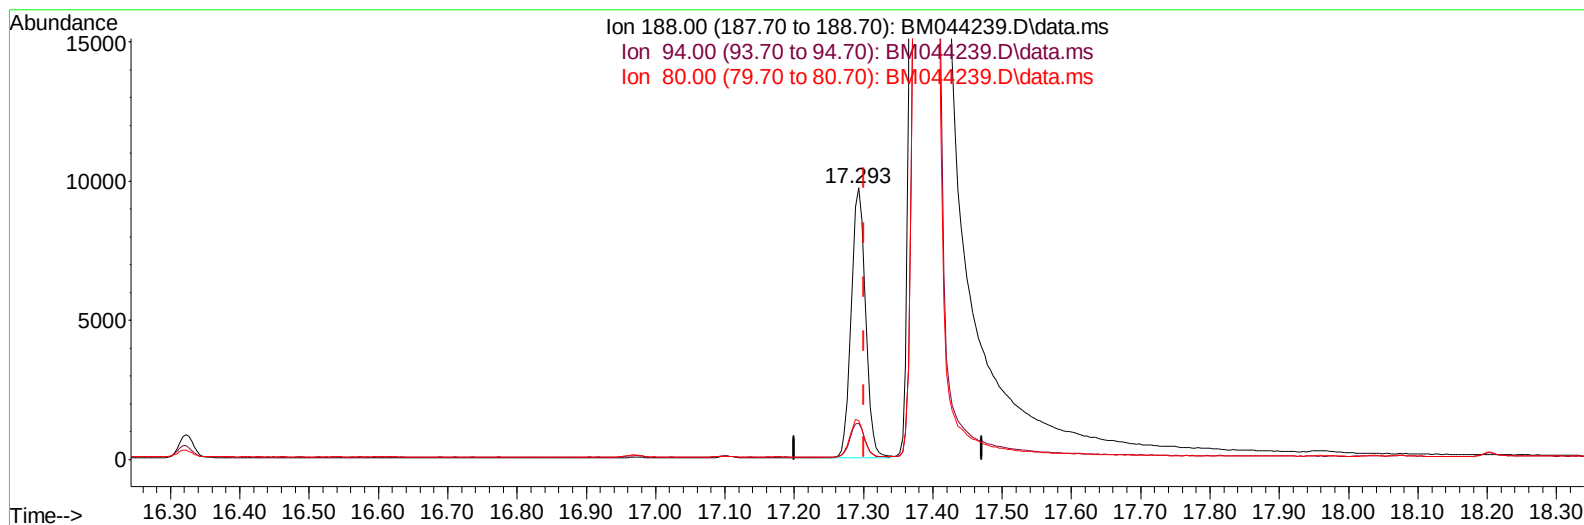

TIC: BM044239.D\data.ms

(13) Phenanthrene-d10 (I)

17.293min (-0.007) 0.40 ng/ul m

response 13917

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.40	13.27
80.00	13.40	14.31
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022124\
Data File : BM044239.D
Acq On : 22 Feb 2024 14:30
Operator : MA/JU
Sample : P1494-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3Y4

Manual IntegrationsAPPROVED

Quant Time: Feb 22 15:07:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/22/2024
Supervised By :mohammad ahmed 02/23/2024

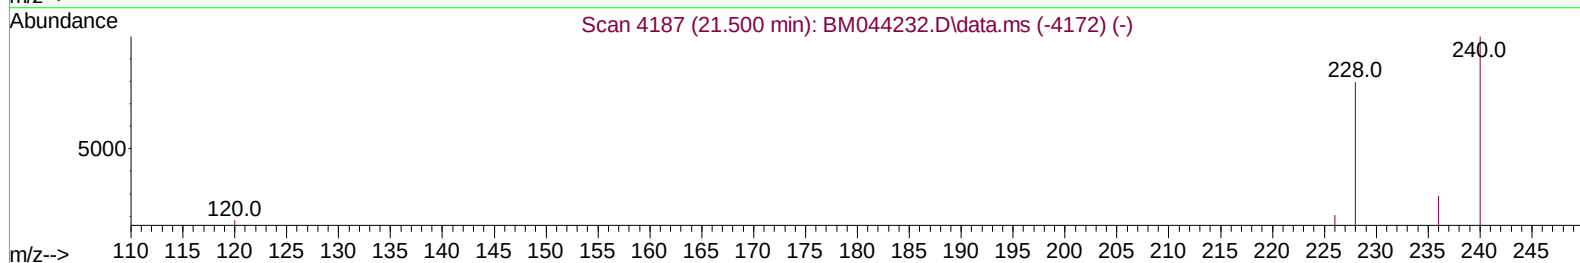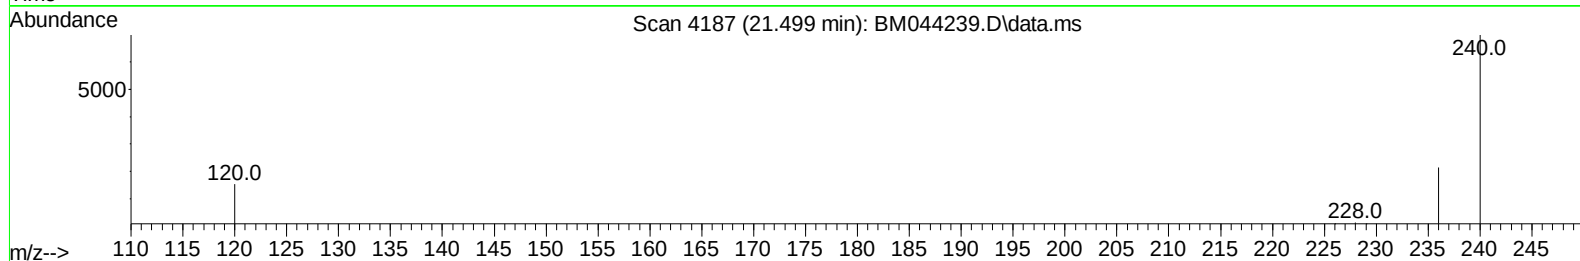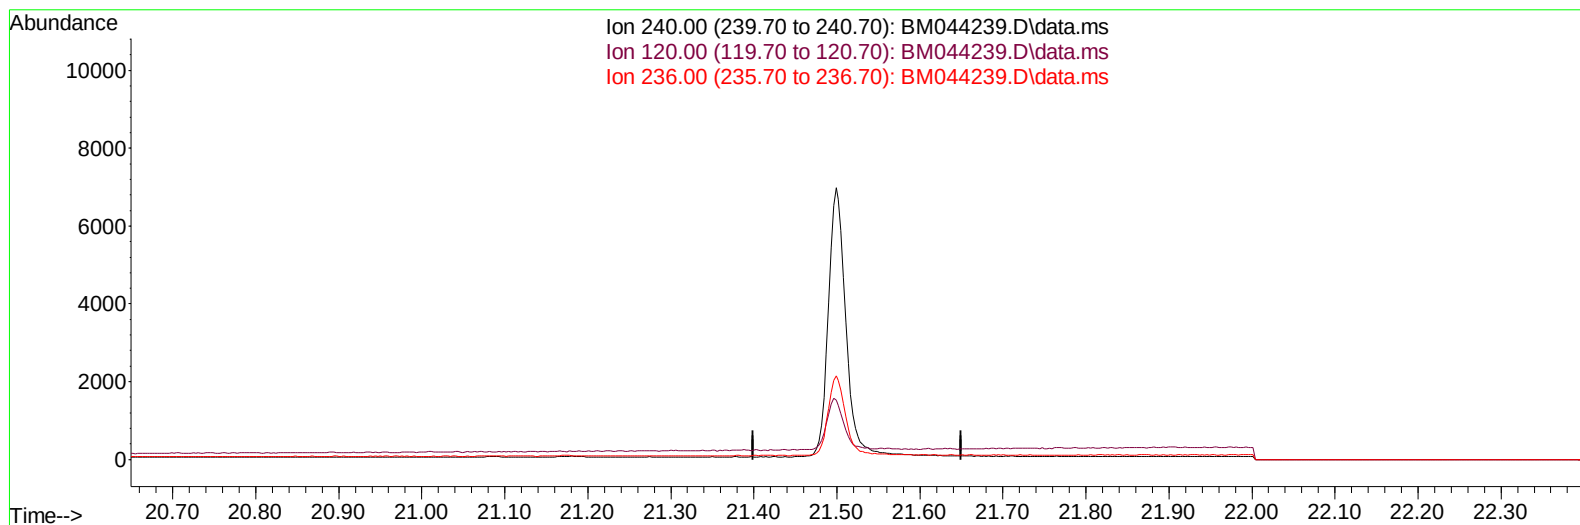

TIC: BM044239.D\data.ms

(17) Chrysene-d12

21.500min (-21.500) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	20.50	0.00#
236.00	30.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022124\
Data File : BM044239.D
Acq On : 22 Feb 2024 14:30
Operator : MA/JU
Sample : P1494-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3Y4

Manual IntegrationsAPPROVED

Quant Time: Feb 22 15:07:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/22/2024
Supervised By :mohammad ahmed 02/23/2024

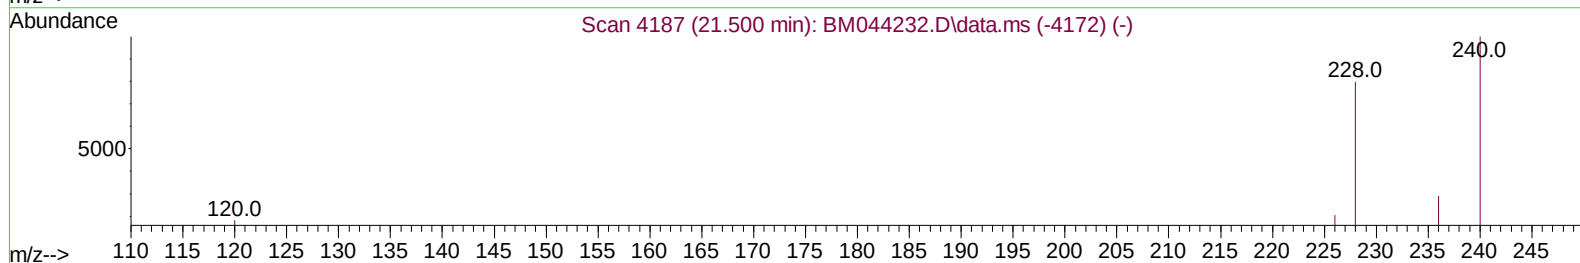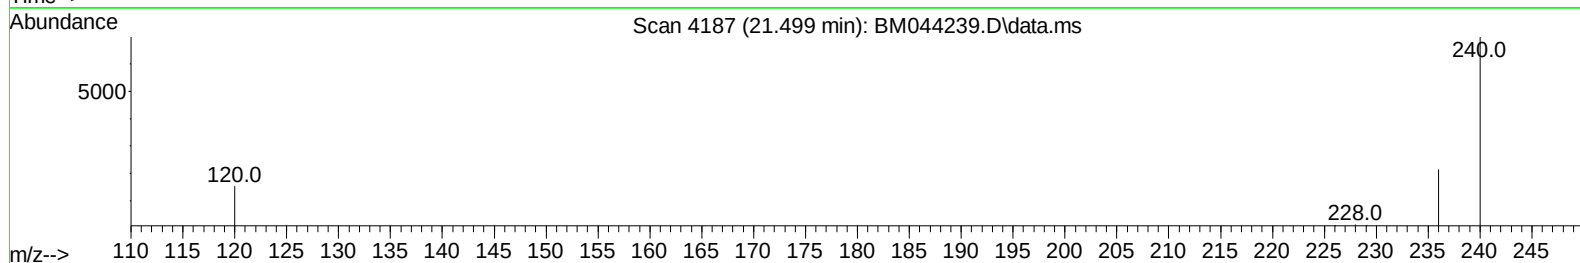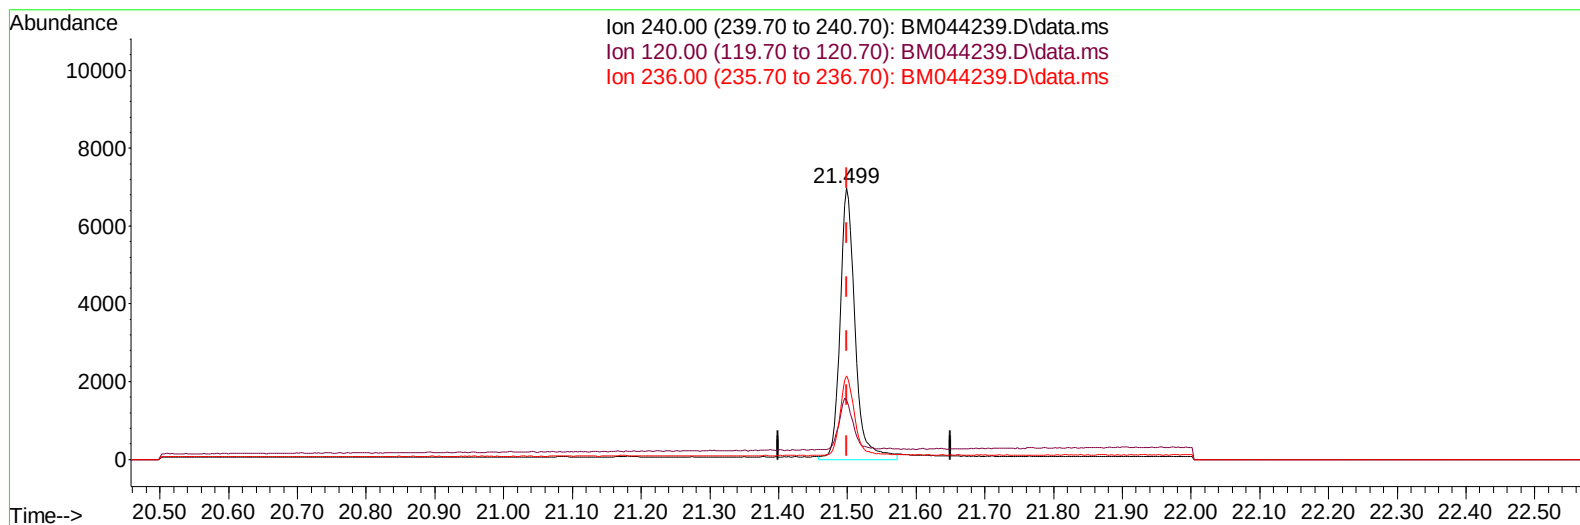

TIC: BM044239.D\data.ms

(17) Chrysene-d12

21.499min (-0.001) 0.40 ng/ul m

response 10607

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.50	21.85
236.00	30.60	30.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022124\
 Data File : BM044239.D
 Acq On : 22 Feb 2024 14:30
 Operator : MA/JU
 Sample : P1494-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3Y4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/22/2024
 Supervised By :mohammad ahmed 02/23/2024

Quant Time: Feb 22 15:07:26 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 15 13:40:24 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.896	152		4382	0.400	ng/ul	0.00
4) Naphthalene-d8	10.693	136		13491	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.539	164		6656	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.293	188		13917m	0.400	ng/ul	0.00
17) Chrysene-d12	21.499	240		10607m	0.400	ng/ul	0.00
23) Perylene-d12	23.884	264		18974	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.348	96		29175	4.701	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.288	152		7873	0.417	ng/ul	-0.01
18) Fluoranthene-d10	19.327	212		16497	0.521	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.382	88		293	0.047	ng/ul#	67

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022124\
Data File : BM044239.D
Acq On : 22 Feb 2024 14:30
Operator : MA/JU
Sample : P1494-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3Y4

Manual IntegrationsAPPROVED

Quant Time: Feb 22 15:07:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/22/2024
Supervised By :mohammad ahmed 02/23/2024

