

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022124\
 Data File : BM044238.D
 Acq On : 22 Feb 2024 13:54
 Operator : MA/JU
 Sample : P1493-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3Y8

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/22/2024
 Supervised By :mohammad ahmed 02/23/2024

Quant Time: Feb 22 14:22:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 15 13:40:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.896	152	5340	0.400	ng/ul	0.00
4) Naphthalene-d8	10.693	136	16178	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.538	164	7903	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.292	188	15984m	0.400	ng/ul	0.00
17) Chrysene-d12	21.500	240	11175m	0.400	ng/ul	0.00
23) Perylene-d12	23.888	264	18726	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.348	96	34676	4.585	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.288	152	9885	0.436	ng/ul	-0.01
18) Fluoranthene-d10	19.326	212	17841	0.535	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.382	88	651	0.086	ng/ul#	62

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022124\
Data File : BM044238.D
Acq On : 22 Feb 2024 13:54
Operator : MA/JU
Sample : P1493-15
Misc :
ALS Vial : 26 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BH3Y8

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 02/22/2024
Supervised By :mohammad ahmed 02/23/2024


Quant Time: Feb 22 14:22:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

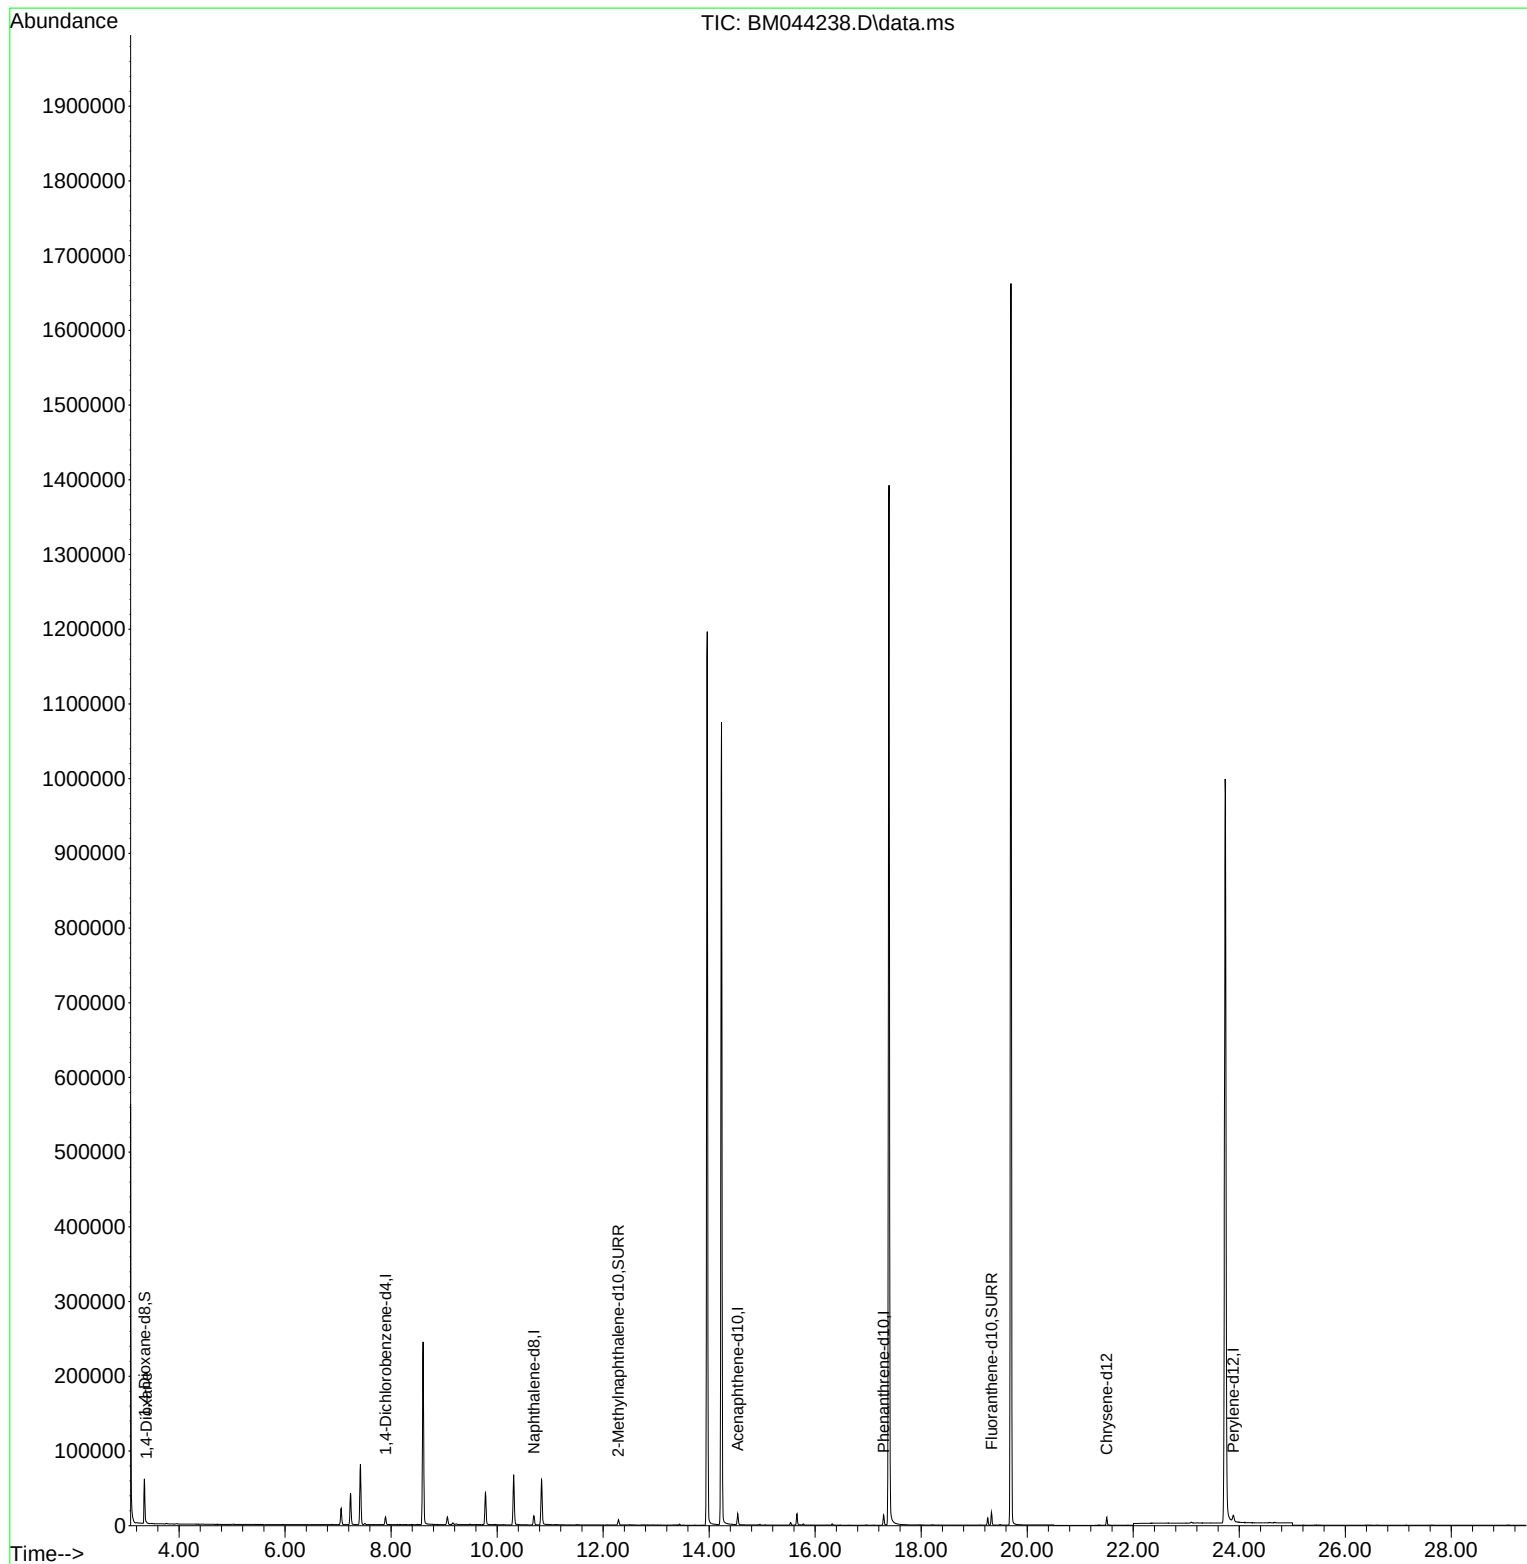

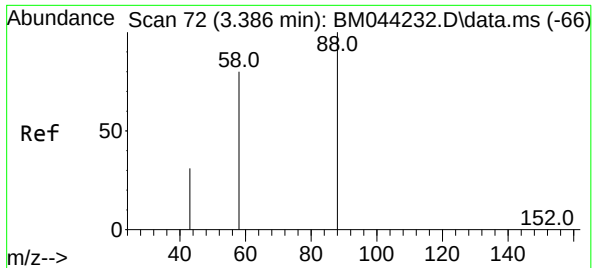

#2
 1,4-Dioxane
 Concen: 0.086 ng/ul
 RT: 3.382 min Scan# 71
 Delta R.T. -0.008 min
 Lab File: BM044238.D
 Acq: 22 Feb 2024 13:54

Instrument :
 BNA_M
 ClientSampleId :
 BH3Y8

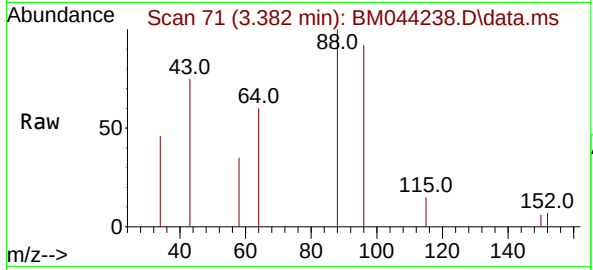

Tgt Ion: 88 Resp: 65

Ion	Ratio	Lower	Upper
88	100		
43	75.4	32.2	48.2
58	34.7	40.6	60.8

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/22/2024
 Supervised By :mohammad ahmed 02/23/2024

