

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022216\
 Data File : BM004335.D
 Acq On : 23 Feb 2016 05:33
 Operator : SJ/UM
 Sample : H1499-29
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-S24-0003

Quant Time: Feb 23 07:08:11 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 23 07:03:02 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	36017	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	171105	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	104521	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	233496	20.00	ng/ul	0.00
78) Chrysene-d12	21.25	240	200072	20.00	ng/ul	0.00
86) Perylene-d12	23.47	264	165455	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.08	96	4158	6.08	ng/uL	0.00
5) Phenol-d5	6.81	99	84874	28.10	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	49829	32.44	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	80145	30.77	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	79312	29.39	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	40762	31.31	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	47072	31.72	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	76366	28.47	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	120193	35.95	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	284162	31.70	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	339394	32.34	ng/ul	0.00
52) 4-Nitrophenol-d4	14.53	143	33117	22.98	ng/ul	0.00
58) Fluorene-d10	15.29	176	239778	31.45	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.43	200	35336	24.64	ng/ul	0.00
71) Anthracene-d10	17.14	188	367972	32.16	ng/ul	0.00
79) Pyrene-d10	19.44	212	388477	40.14	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.33	264	287278	33.09	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.75	163	98932	10.58	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022216\
Data File : BM004335.D
Acq On : 23 Feb 2016 05:33
Operator : SJ/UM
Sample : H1499-29
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0311-S24-0003

Quant Time: Feb 23 07:08:11 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 23 07:03:02 2016
Response via : Initial Calibration

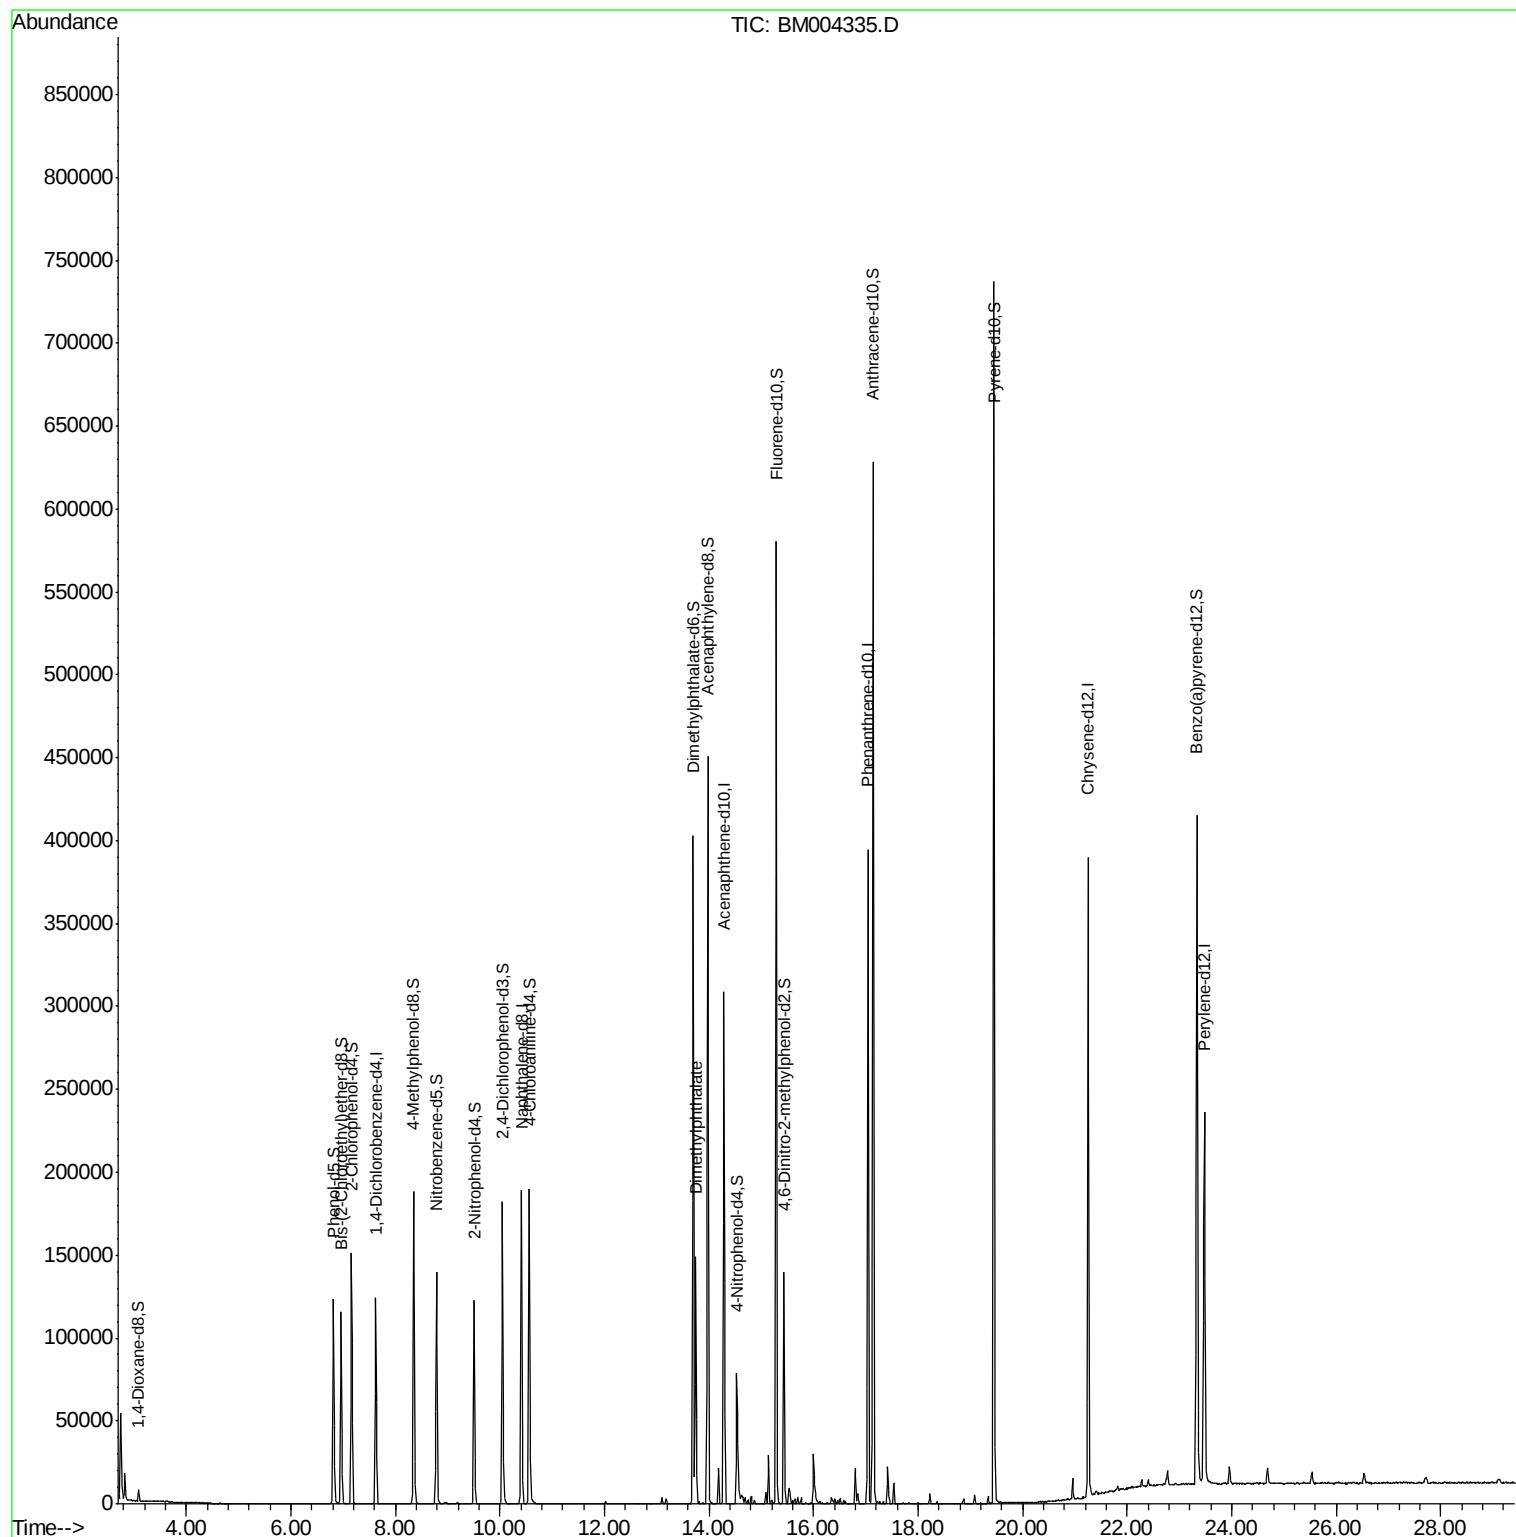

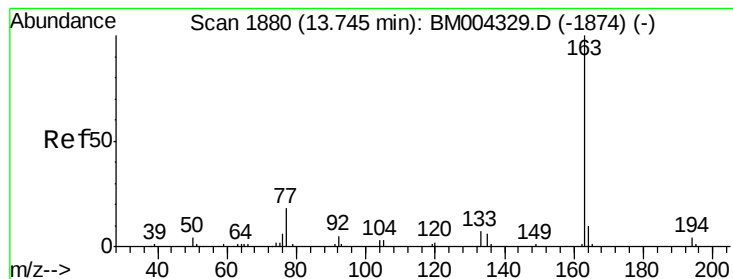

#45

Dimethylphthalate

Concen: 10.58 ng/ul

RT: 13.75 min Scan# 1880

Delta R.T. 0.00 min

Lab File: BM004335.D


Acq: 23 Feb 2016 05:33

Instrument :

BNA_M

ClientSampleId :

0311-S24-0003

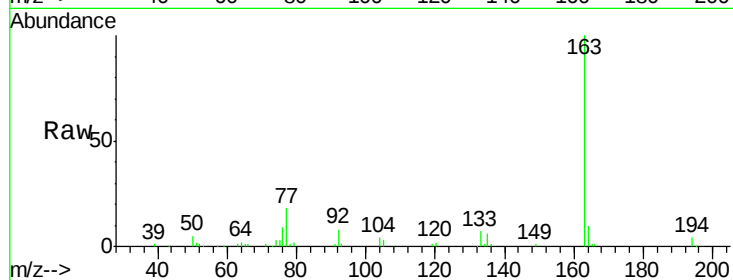

Tgt Ion:163 Resp: 98932

Ion Ratio Lower Upper

163 100

194 4.0 3.2 4.8

164 9.9 7.8 11.8

