

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM022216\
 Data File : BM004323.D
 Acq On : 22 Feb 2016 22:20
 Operator : SJ/UM
 Sample : H1499-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Feb 23 00:16:07 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 23 00:11:03 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 0311-S10-0003

Manual Integrations
 APPROVED

Sohil
 2/23/2016 5:23:25 PM

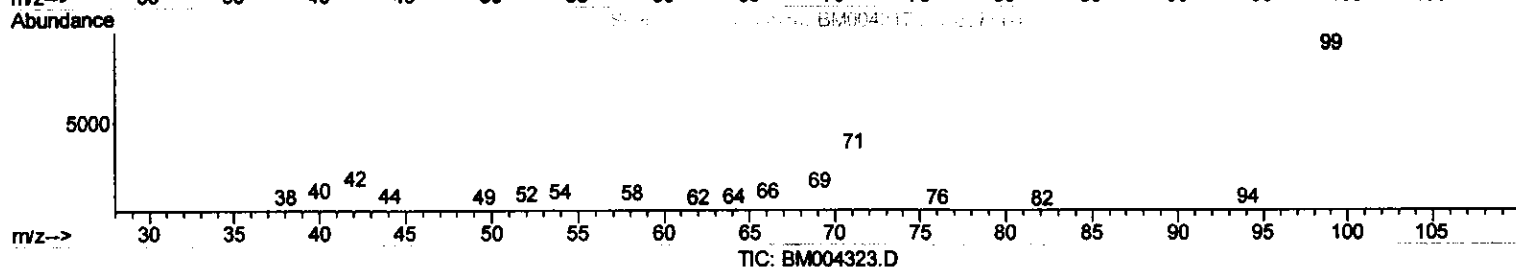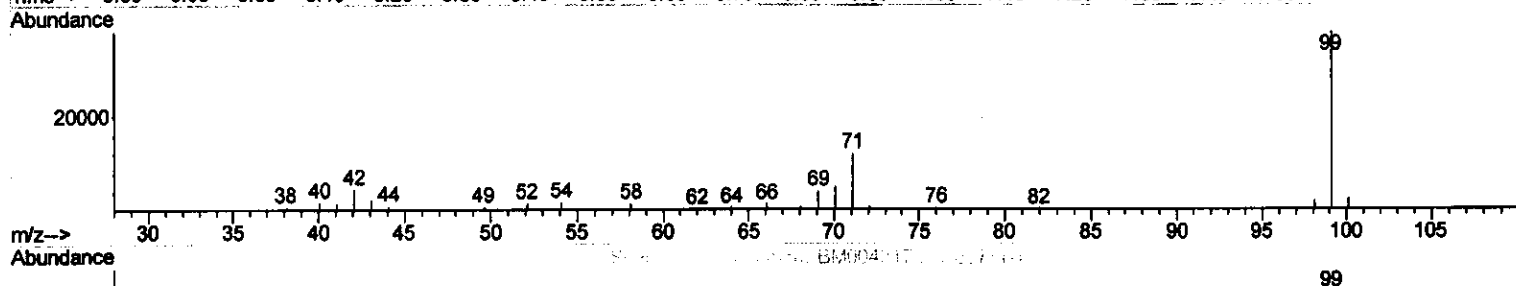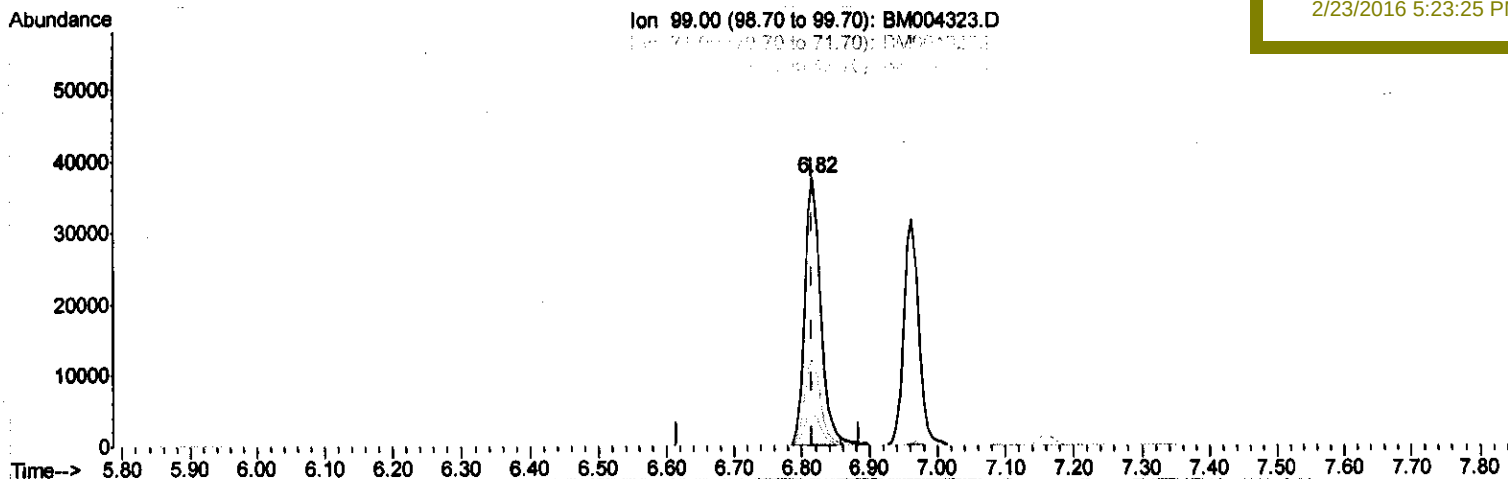

(5) Phenol-d5 (S)

6.816min (-0.000) 25.59ng/ul

response 60201

Ion	Exp%	Act%
99.00	100	100
71.00	35.10	32.29
42.00	14.10	12.57
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM022216\
 Data File : BM004323.D
 Acq On : 22 Feb 2016 22:20
 Operator : SJ/UM
 Sample : H1499-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Feb 23 00:16:07 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 23 00:11:03 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 0311-S10-0003

Manual Integrations
 APPROVED

Sohil
 2/23/2016 5:23:25 PM

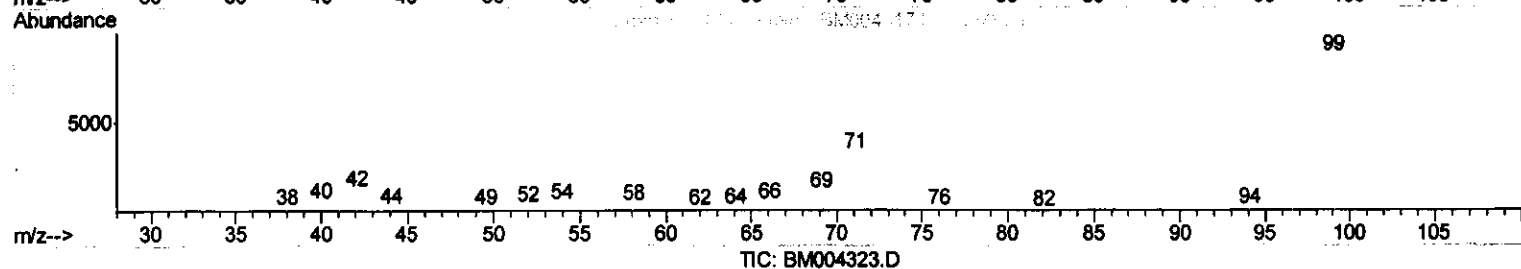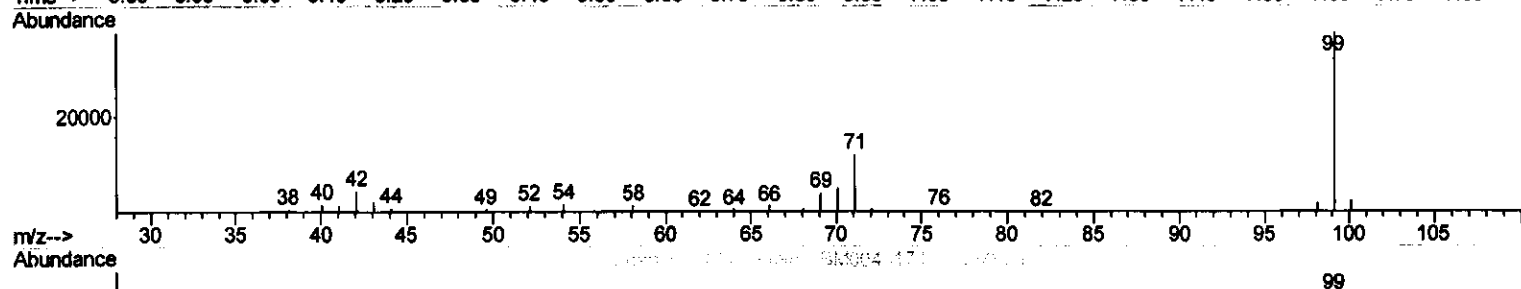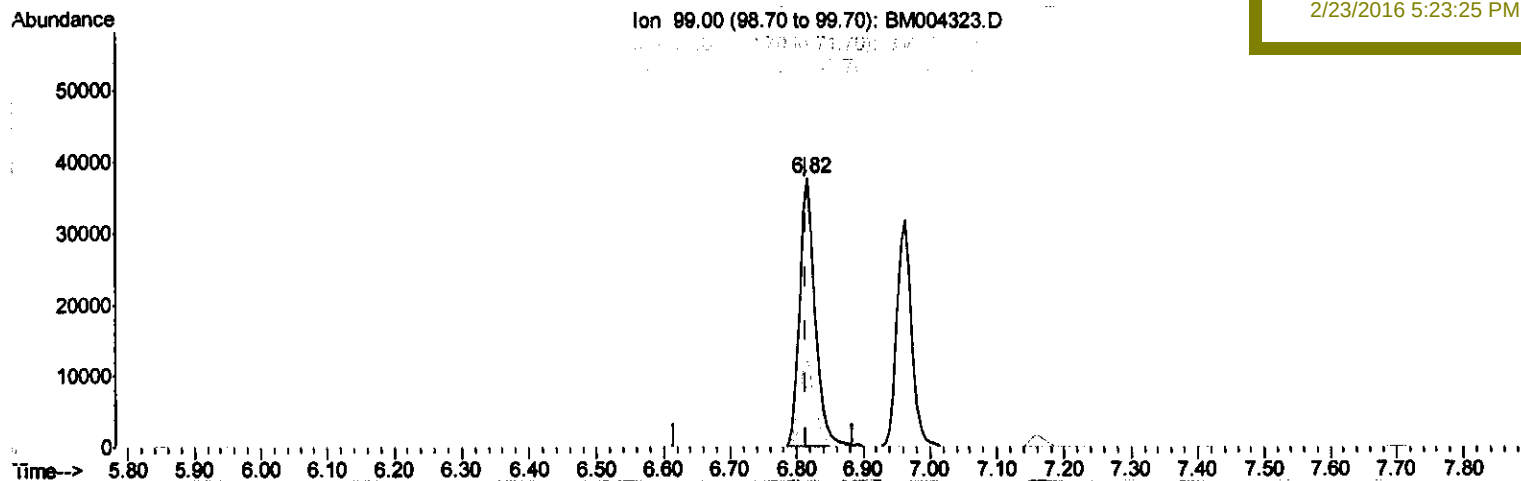

(5) Phenol-d5 (S)

6.816min (-0.000) 25.91ng/ul m

response 60950

Ion	Exp%	Act%
99.00	100	100
71.00	35.10	32.29
42.00	14.10	12.57
0.00	0.00	0.00

> 5.7

2/29/16

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM022216\
 Data File : BM004323.D
 Acq On : 22 Feb 2016 22:20
 Operator : SJ/UM
 Sample : H1499-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Feb 23 00:16:07 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 23 00:11:03 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 0311-S10-0003

Manual Integrations
 APPROVED

Sohil
 2/23/2016 5:23:25 PM

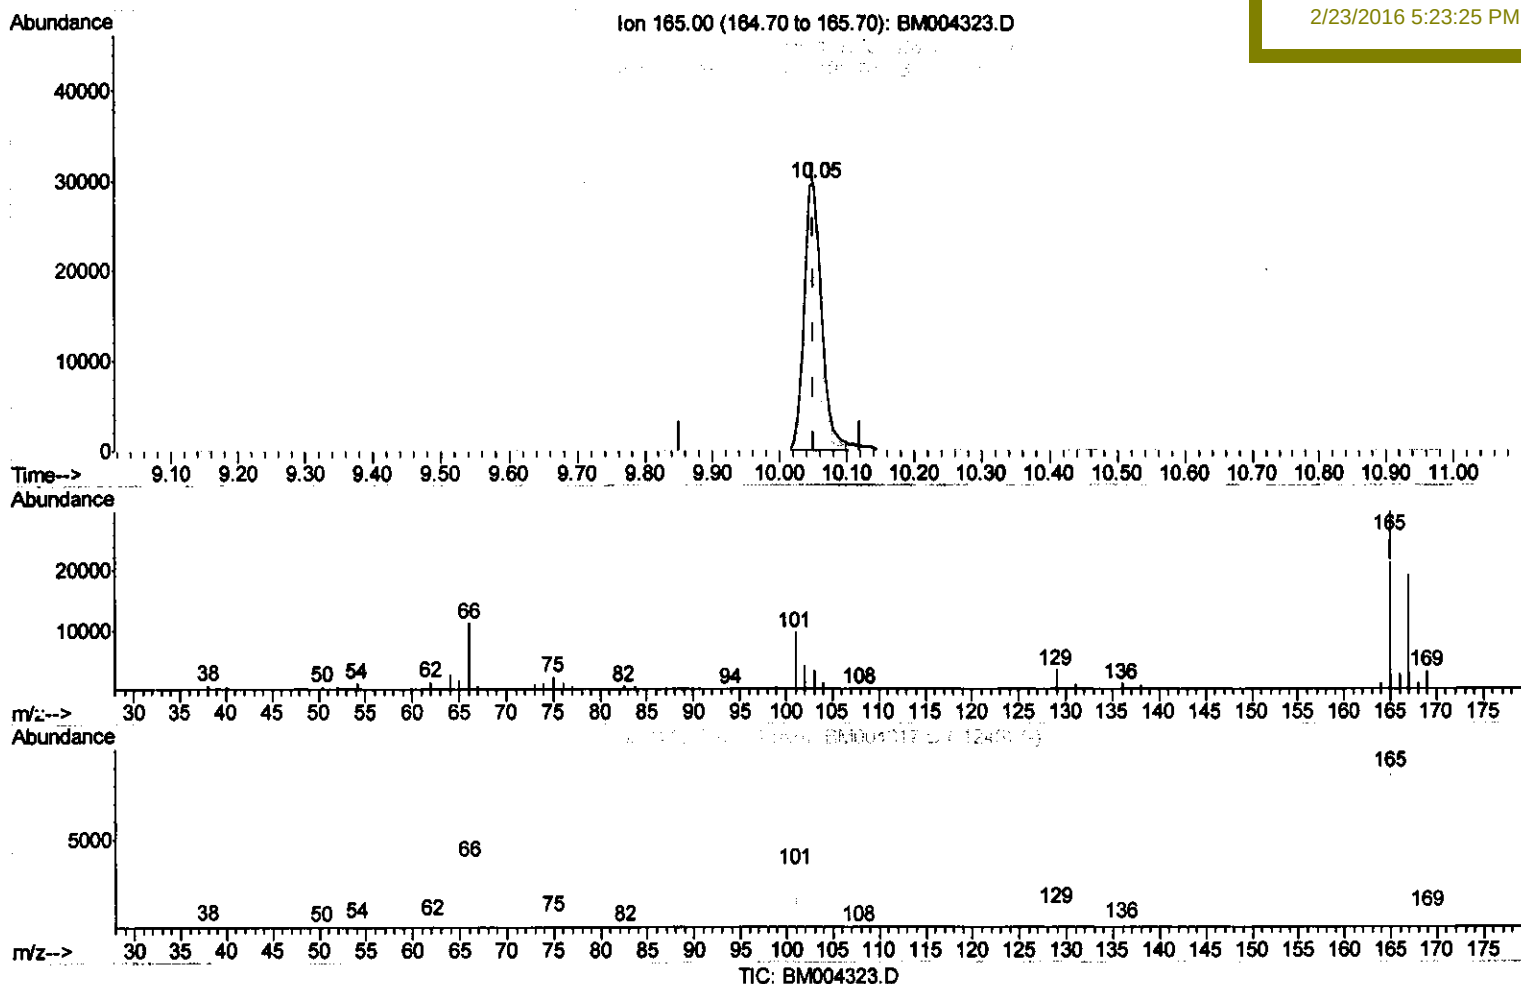

(26) 2,4-Dichlorophenol-d3 (S)

10.051min (-0.000) 25.44ng/ul

response 53651

Ion	Exp%	Act%
165.00	100	100
167.00	65.30	64.55
101.00	34.20	32.74
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM022216\
 Data File : BM004323.D
 Acq On : 22 Feb 2016 22:20
 Operator : SJ/UM
 Sample : H1499-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Feb 23 00:16:07 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 23 00:11:03 2016
 Response via : Initial Calibration

Instrument :
 BNA M
 ClientSampleId :
 0311-S10-0003

Manual Integrations
 APPROVED

Sohil
 2/23/2016 5:23:25 PM

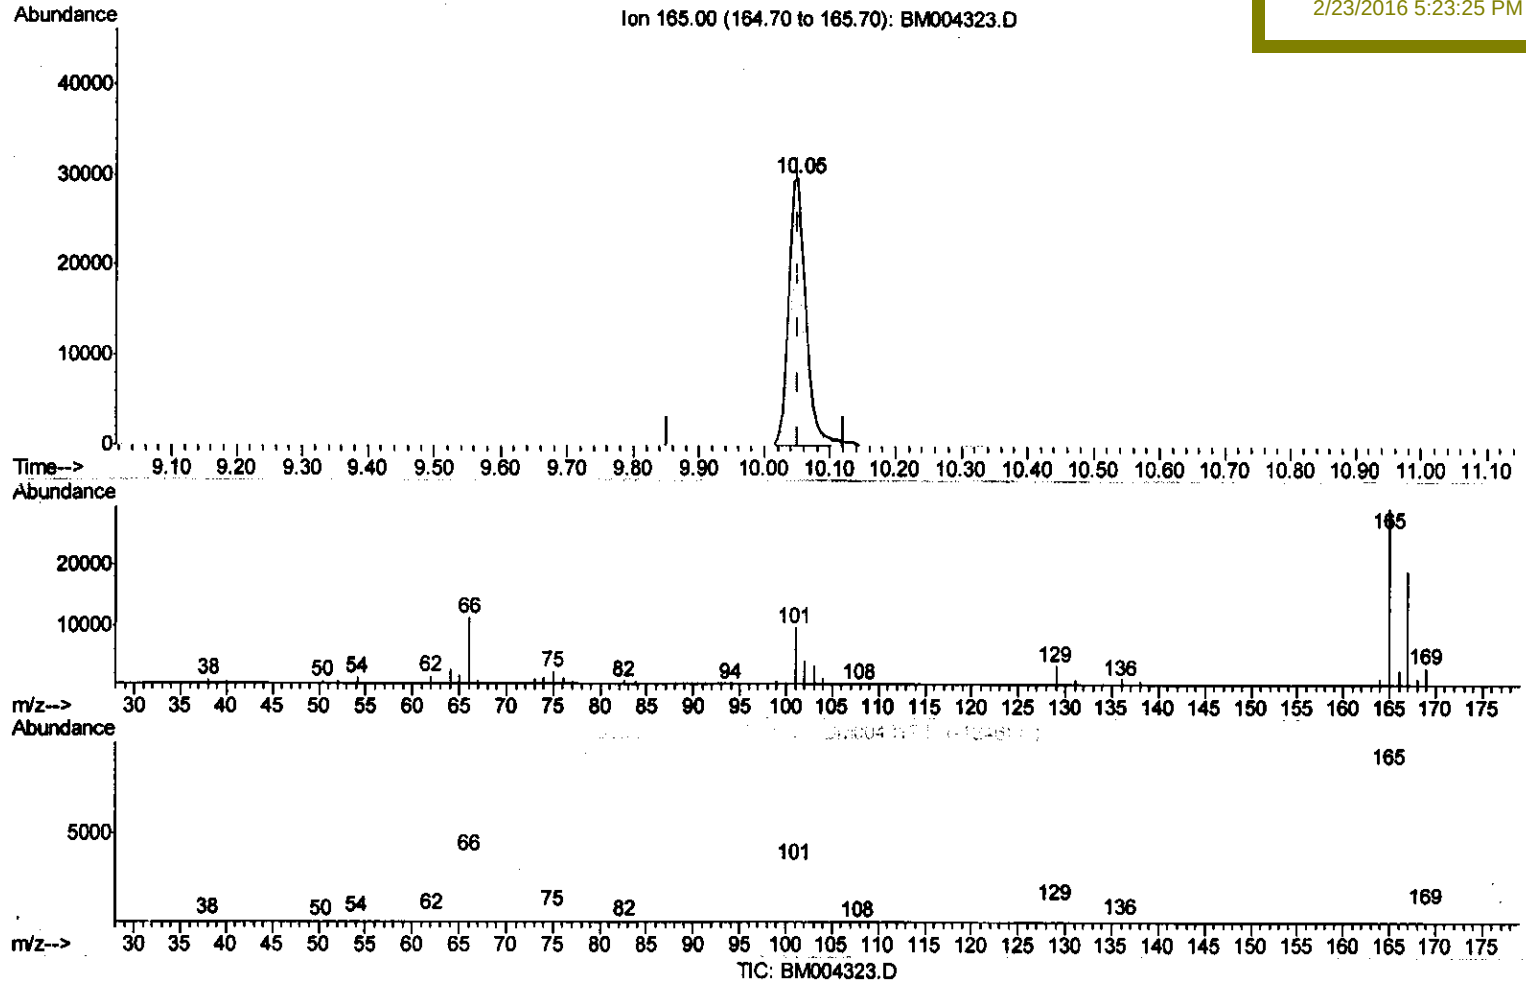

(26) 2,4-Dichlorophenol-d3 (S)

10.051min (-0.000) 26.00ng/ul m

response 54827

Ion	Exp%	Act%
165.00	100	100
167.00	65.30	64.55
101.00	34.20	32.74
0.00	0.00	0.00

5.3
 2/29/16

Data Path : Z:\HPCHEM1\BNA_M\Data\BM022216\
 Data File : BM004323.D
 Acq On : 22 Feb 2016 22:20
 Operator : SJ/UM
 Sample : H1499-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-S10-0003

Quant Time: Feb 23 00:46:47 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 23 00:11:03 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 2/23/2016 5:23:25 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	28057	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	134536	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	85414	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	202702	20.00	ng/ul	0.00
78) Chrysene-d12	21.25	240	239144	20.00	ng/ul	0.00
86) Perylene-d12	23.47	264	228005	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.08	96	2689	5.05	ng/uL	0.00
5) Phenol-d5	6.82	99	60950m	25.91	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	33815	28.26	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	54409	26.81	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	55499	26.40	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	27726	27.09	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	32379	27.75	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	54827m	26.00	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	83132	31.63	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	215883	29.47	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	246102	28.70	ng/ul	0.00
52) 4-Nitrophenol-d4	14.53	143	27251	23.14	ng/ul	0.00
58) Fluorene-d10	15.29	176	182305	29.26	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.43	200	25354	20.36	ng/ul	0.00
71) Anthracene-d10	17.14	188	294304	29.63	ng/ul	0.00
79) Pyrene-d10	19.44	212	343157	29.66	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.33	264	358236	29.94	ng/ul	0.00

9.9
 2/29/16

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.74	163	87350	11.44	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\Data\BM022216\
Data File : BM004323.D
Acq On : 22 Feb 2016 22:20
Operator : SJ/UM
Sample : H1499-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Feb 23 00:46:47 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 23 00:11:03 2016
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
0311-S10-0003

Manual Integrations
APPROVED

Sohil
2/23/2016 5:23:25 PM

