

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022216\
 Data File : BM004319.D
 Acq On : 22 Feb 2016 19:55
 Operator : SJ/UM
 Sample : H1499-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-SS01A

Manual Integrations
 APPROVED

Sohil
 2/23/2016 5:23:08 PM

Quant Time: Feb 23 10:44:27 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM022216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 23 07:03:02 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	23717	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	116092	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	74662	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	177684	20.00	ng/ul	0.00
78) Chrysene-d12	21.25	240	213509	20.00	ng/ul	0.00
86) Perylene-d12	23.47	264	211127	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.09	96	2014	4.48	ng/uL	0.00
5) Phenol-d5	6.82	99	46632m	23.45	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	26185	25.89	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	42025	24.50	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	42144	23.72	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	21436	24.27	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	24824	24.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	42570m	23.39	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	63546	28.02	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	170748	26.67	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	195560	26.09	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	23978	23.30	ng/ul	0.00
58) Fluorene-d10	15.29	176	145347	26.69	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.43	200	21953	20.11	ng/ul	0.00
71) Anthracene-d10	17.14	188	234979	26.99	ng/ul	0.00
79) Pyrene-d10	19.44	212	278929	27.01	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.33	264	303065	27.35	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.74	163	70471	10.55	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM022216\
Data File : BM004319.D
Acq On : 22 Feb 2016 19:55
Operator : SJ/UM
Sample : H1499-01
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
0311-SS01A

Manual Integrations
APPROVED

Sohil
2/23/2016 5:23:08 PM

Quant Time: Feb 23 10:44:27 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 23 07:03:02 2016
Response via : Initial Calibration

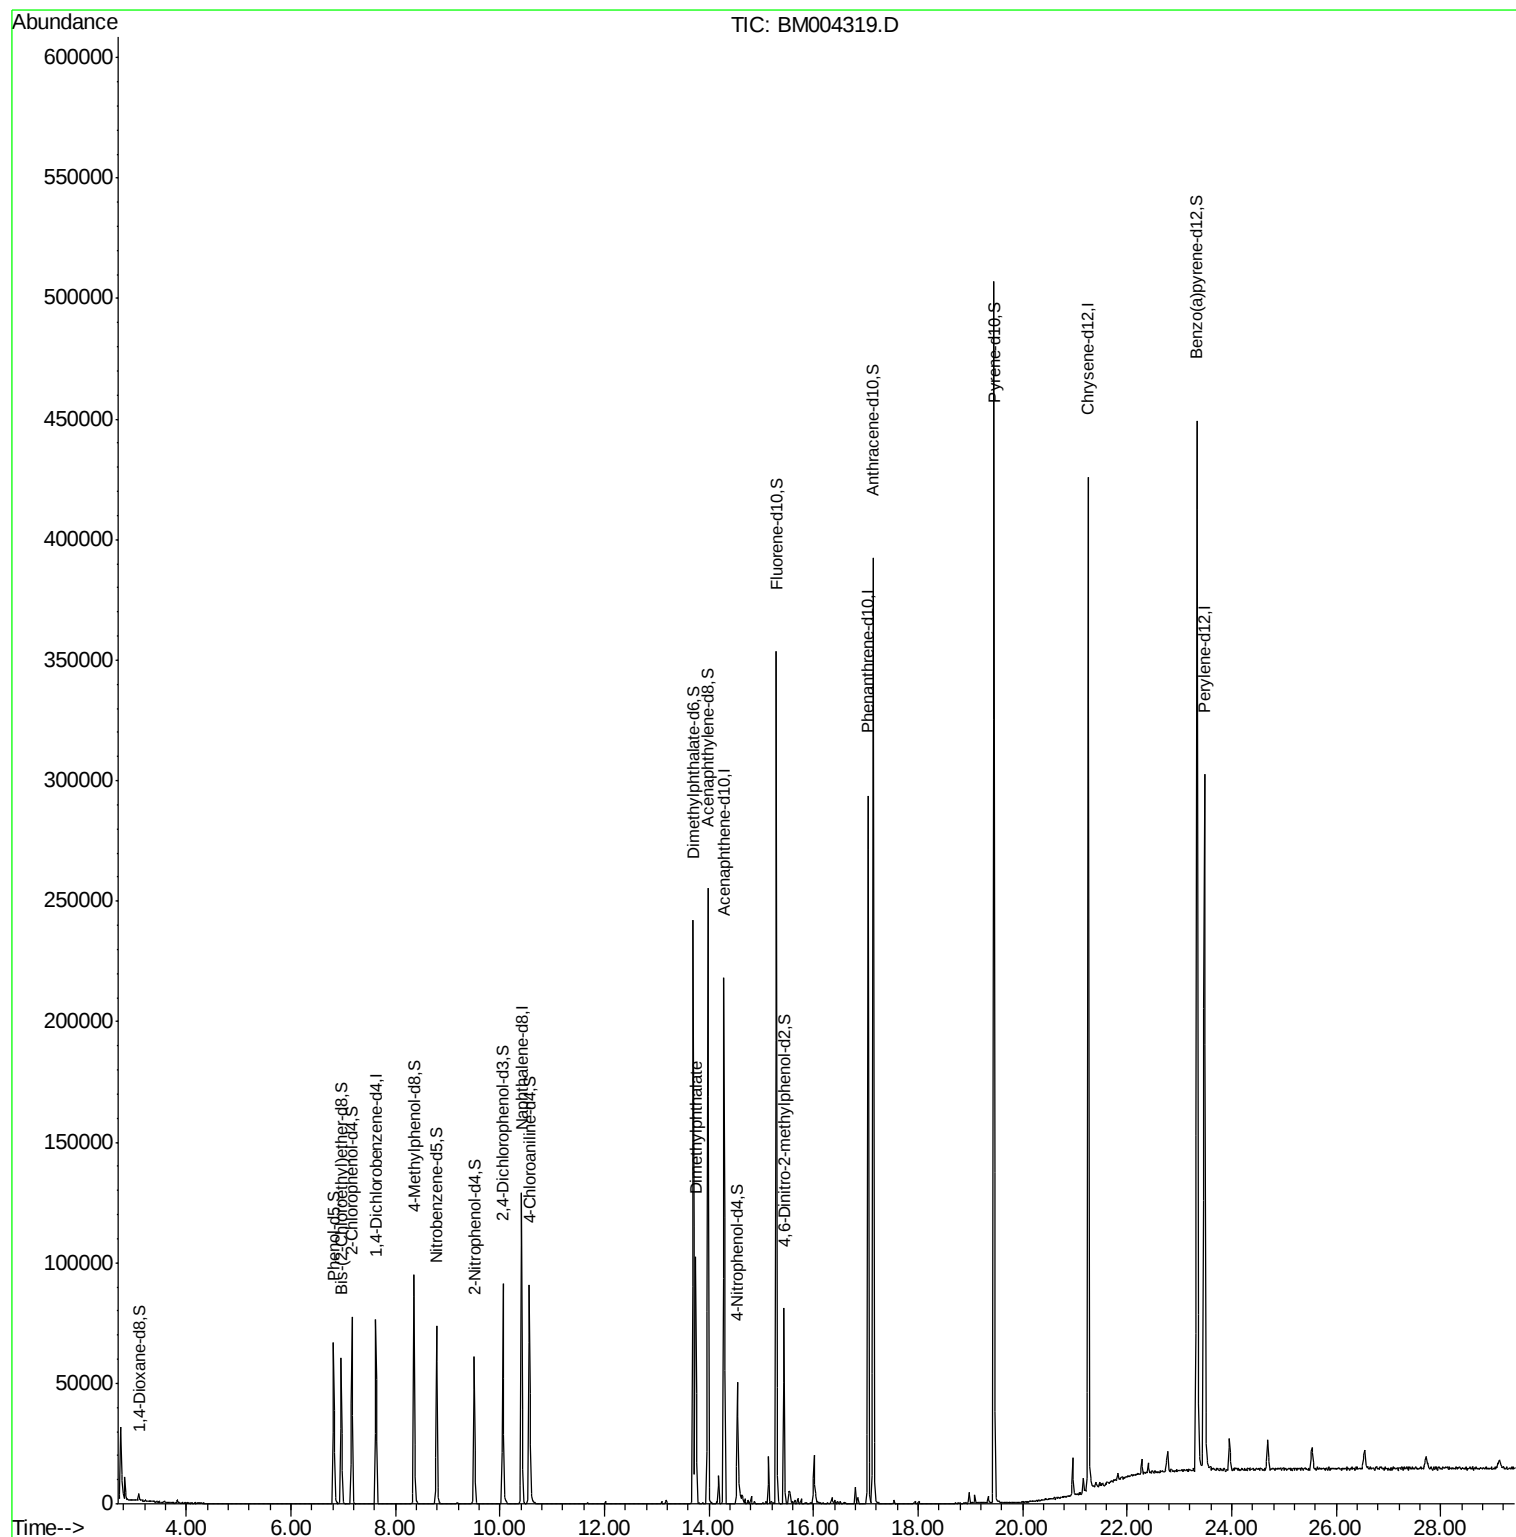

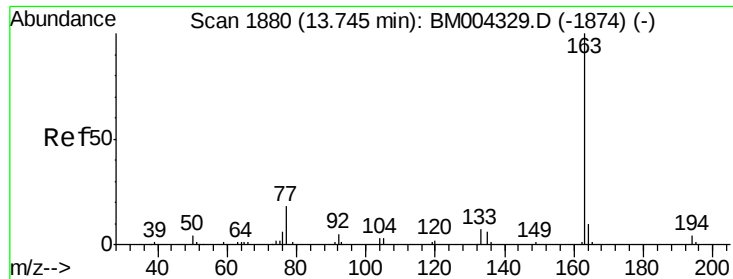

#45
 Dimethylphthalate
 Concen: 10.55 ng/ul
 RT: 13.74 min Scan# 1880
 Delta R.T. -0.00 min
 Lab File: BM004319.D
 Acq: 22 Feb 2016 19:55

Instrument :
 BNA_M
 ClientSampleId :
 0311-SS01A

Tot Ion:	163	Resp:	70471
Ion Ratio	Lower	Upper	
163	100		
194	4.3	3.2	4.8
164	10.0	7.8	11.8

Manual Integrations
 APPROVED

Sohil
 2/23/2016 5:23:08 PM

