

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022216\
 Data File : BM004320.D
 Acq On : 22 Feb 2016 20:31
 Operator : SJ/UM
 Sample : H1499-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-SS01B

Manual Integrations
 APPROVED

Sohil
 2/23/2016 5:23:16 PM

Quant Time: Feb 23 00:29:49 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM022216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 23 00:11:03 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	25726	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	124615	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	81407	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	194988	20.00	ng/ul	0.00
78) Chrysene-d12	21.25	240	232114	20.00	ng/ul	0.00
86) Perylene-d12	23.47	264	212813	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.09	96	2143	4.39	ng/uL	0.00
5) Phenol-d5	6.82	99	52616m	24.39	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	29497	26.89	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	47282	25.41	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	50143	26.01	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	25118	26.49	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	28698	26.55	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	49128m	25.15	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	76773	31.53	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	217939	31.22	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	239271	29.27	ng/ul	0.00
52) 4-Nitrophenol-d4	14.53	143	29848	26.60	ng/ul	0.00
58) Fluorene-d10	15.29	176	182521	30.74	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.43	200	29611	24.72	ng/ul	0.00
71) Anthracene-d10	17.14	188	308060	32.24	ng/ul	0.00
79) Pyrene-d10	19.45	212	372549	33.18	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.33	264	386971	34.65	ng/ul	0.00

Target Compounds					Ovalue
45) Dimethylphthalate	13.75	163	79931	10.98	ng/ul 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM022216\
Data File : BM004320.D
Acq On : 22 Feb 2016 20:31
Operator : SJ/UM
Sample : H1499-02
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
0311-SS01B

Manual Integrations
APPROVED

Sohil
2/23/2016 5:23:16 PM

Quant Time: Feb 23 00:29:49 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 23 00:11:03 2016
Response via : Initial Calibration

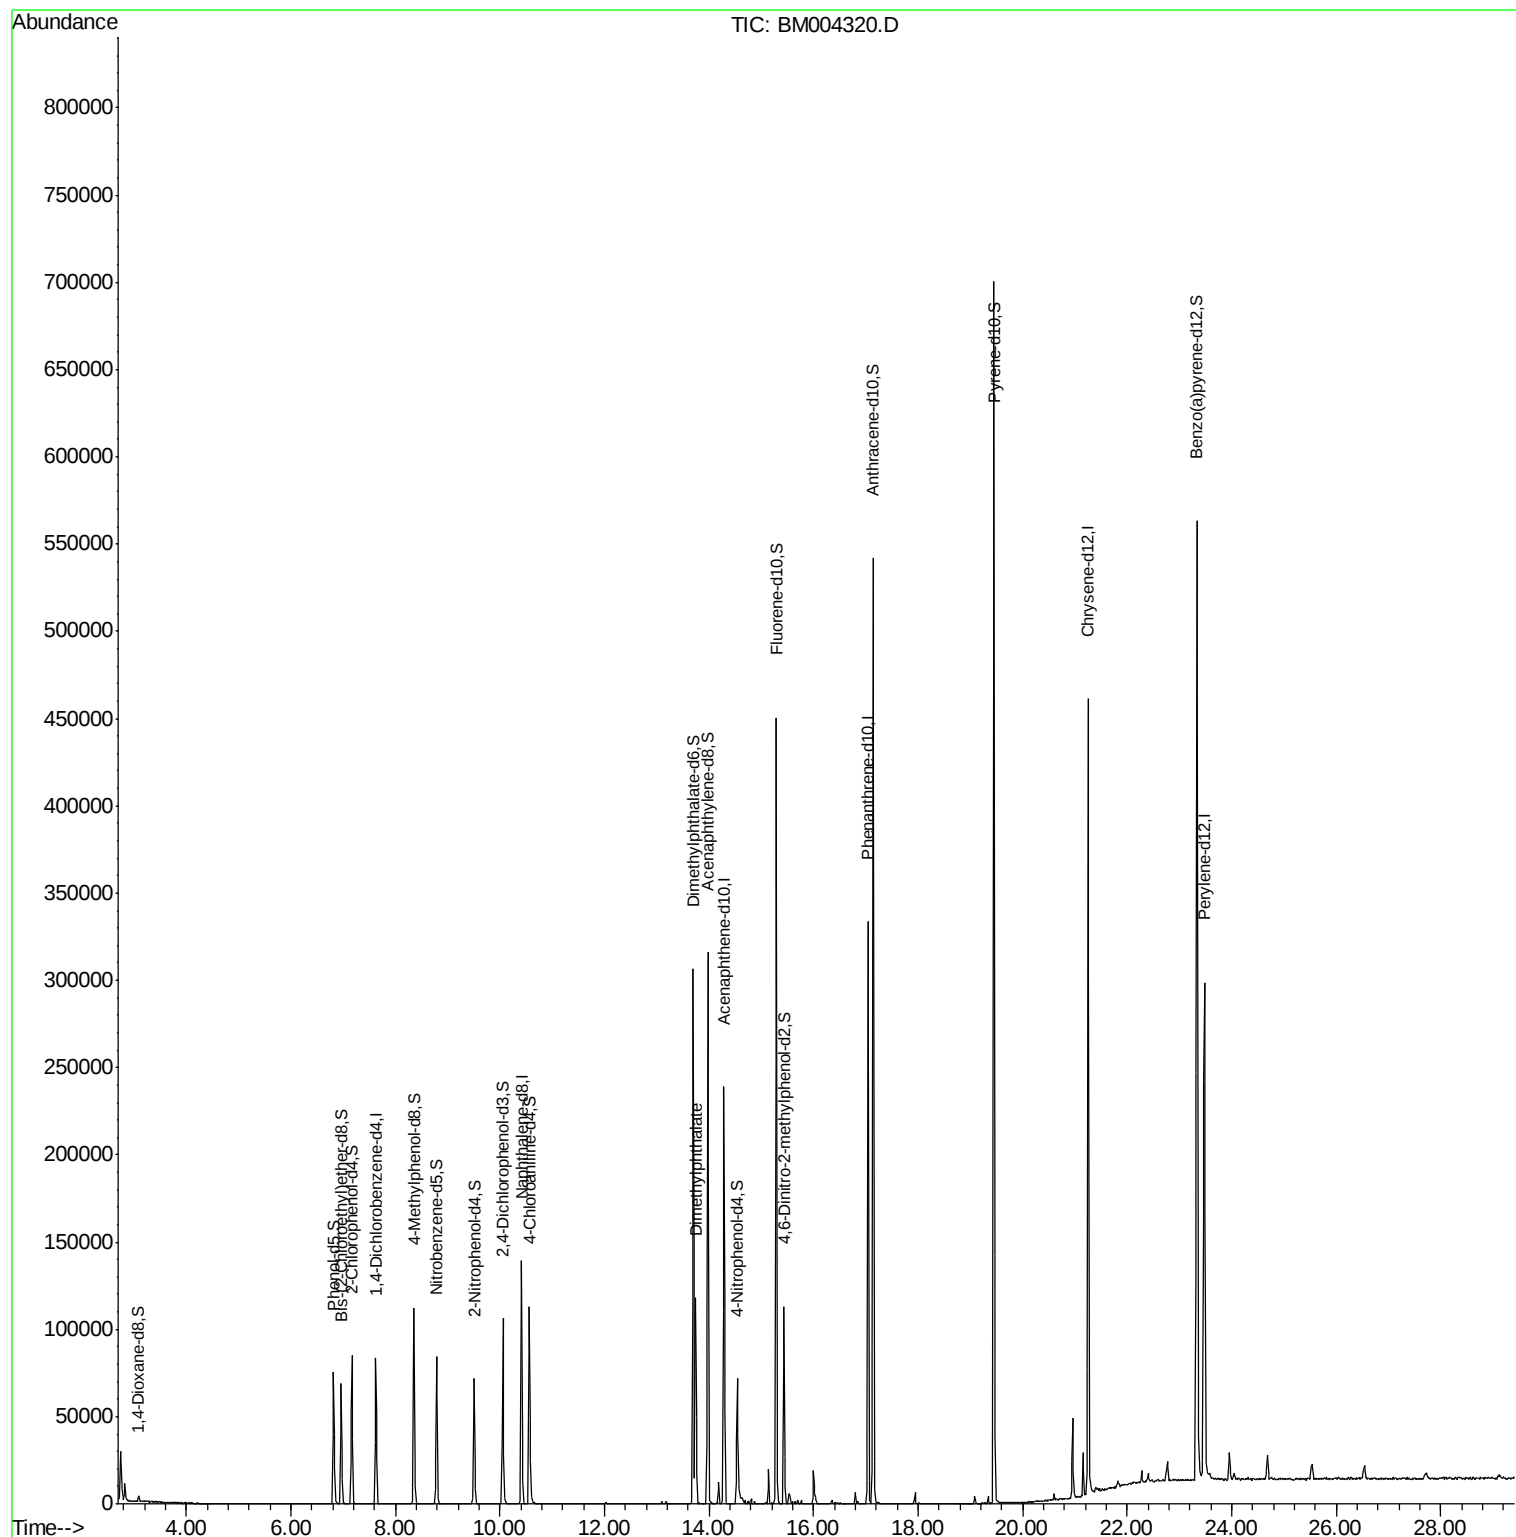

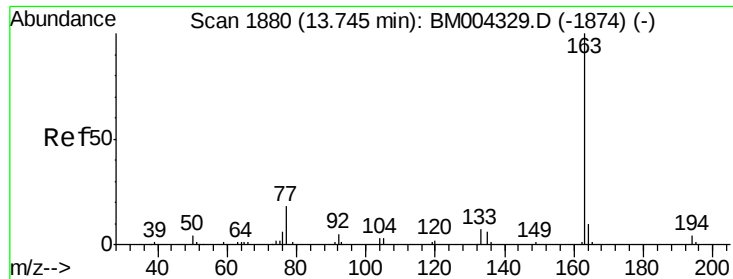

#45

Dimethylphthalate

Concen: 10.98 ng/ul

RT: 13.75 min Scan# 1880

Delta R.T. 0.00 min

Lab File: BM004320.D


Acq: 22 Feb 2016 20:31

Instrument :

BNA_M

ClientSampleId :

0311-SS01B

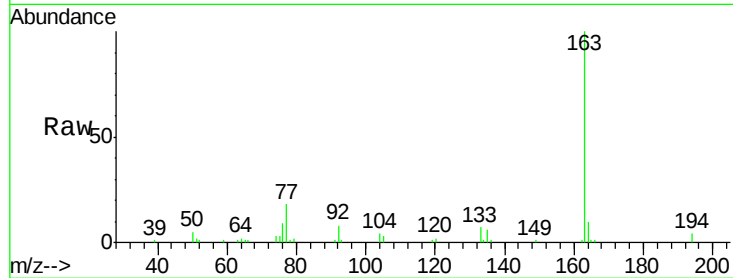

Tot Ion:	163	Resp:	79931
Ion Ratio	Lower	Upper	
163	100		
194	4.2	3.2	4.8
164	10.1	7.8	11.8

Manual Integrations
APPROVED

Sohil
2/23/2016 5:23:16 PM

