

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022216\
 Data File : BM004324.D
 Acq On : 22 Feb 2016 22:56
 Operator : SJ/UM
 Sample : H1499-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-S10-0312

Manual Integrations
 APPROVED

Sohil
 2/23/2016 5:23:31 PM

Quant Time: Feb 23 00:49:46 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM022216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 23 00:11:03 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	25046	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	122382	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	80466	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	195597	20.00	ng/ul	0.00
78) Chrysene-d12	21.25	240	241583	20.00	ng/ul	0.00
86) Perylene-d12	23.47	264	228980	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.08	96	1972	4.15	ng/uL	0.00
5) Phenol-d5	6.82	99	41302m	19.67	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	23867	22.35	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	37664	20.79	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	36486	19.44	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	19132	20.55	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	22064	20.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	37662m	19.63	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	57475	24.04	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	154600	22.40	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	178764	22.13	ng/ul	0.00
52) 4-Nitrophenol-d4	14.53	143	18689	16.85	ng/ul	0.00
58) Fluorene-d10	15.29	176	134810	22.97	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.43	200	19003	15.82	ng/ul	0.00
71) Anthracene-d10	17.14	188	216937	22.64	ng/ul	0.00
79) Pyrene-d10	19.44	212	264785	22.66	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.33	264	279429	23.25	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.75	163	73241	10.18	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM022216\
Data File : BM004324.D
Acq On : 22 Feb 2016 22:56
Operator : SJ/UM
Sample : H1499-07
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
0311-S10-0312

Manual Integrations
APPROVED

Sohil
2/23/2016 5:23:31 PM

Quant Time: Feb 23 00:49:46 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 23 00:11:03 2016
Response via : Initial Calibration

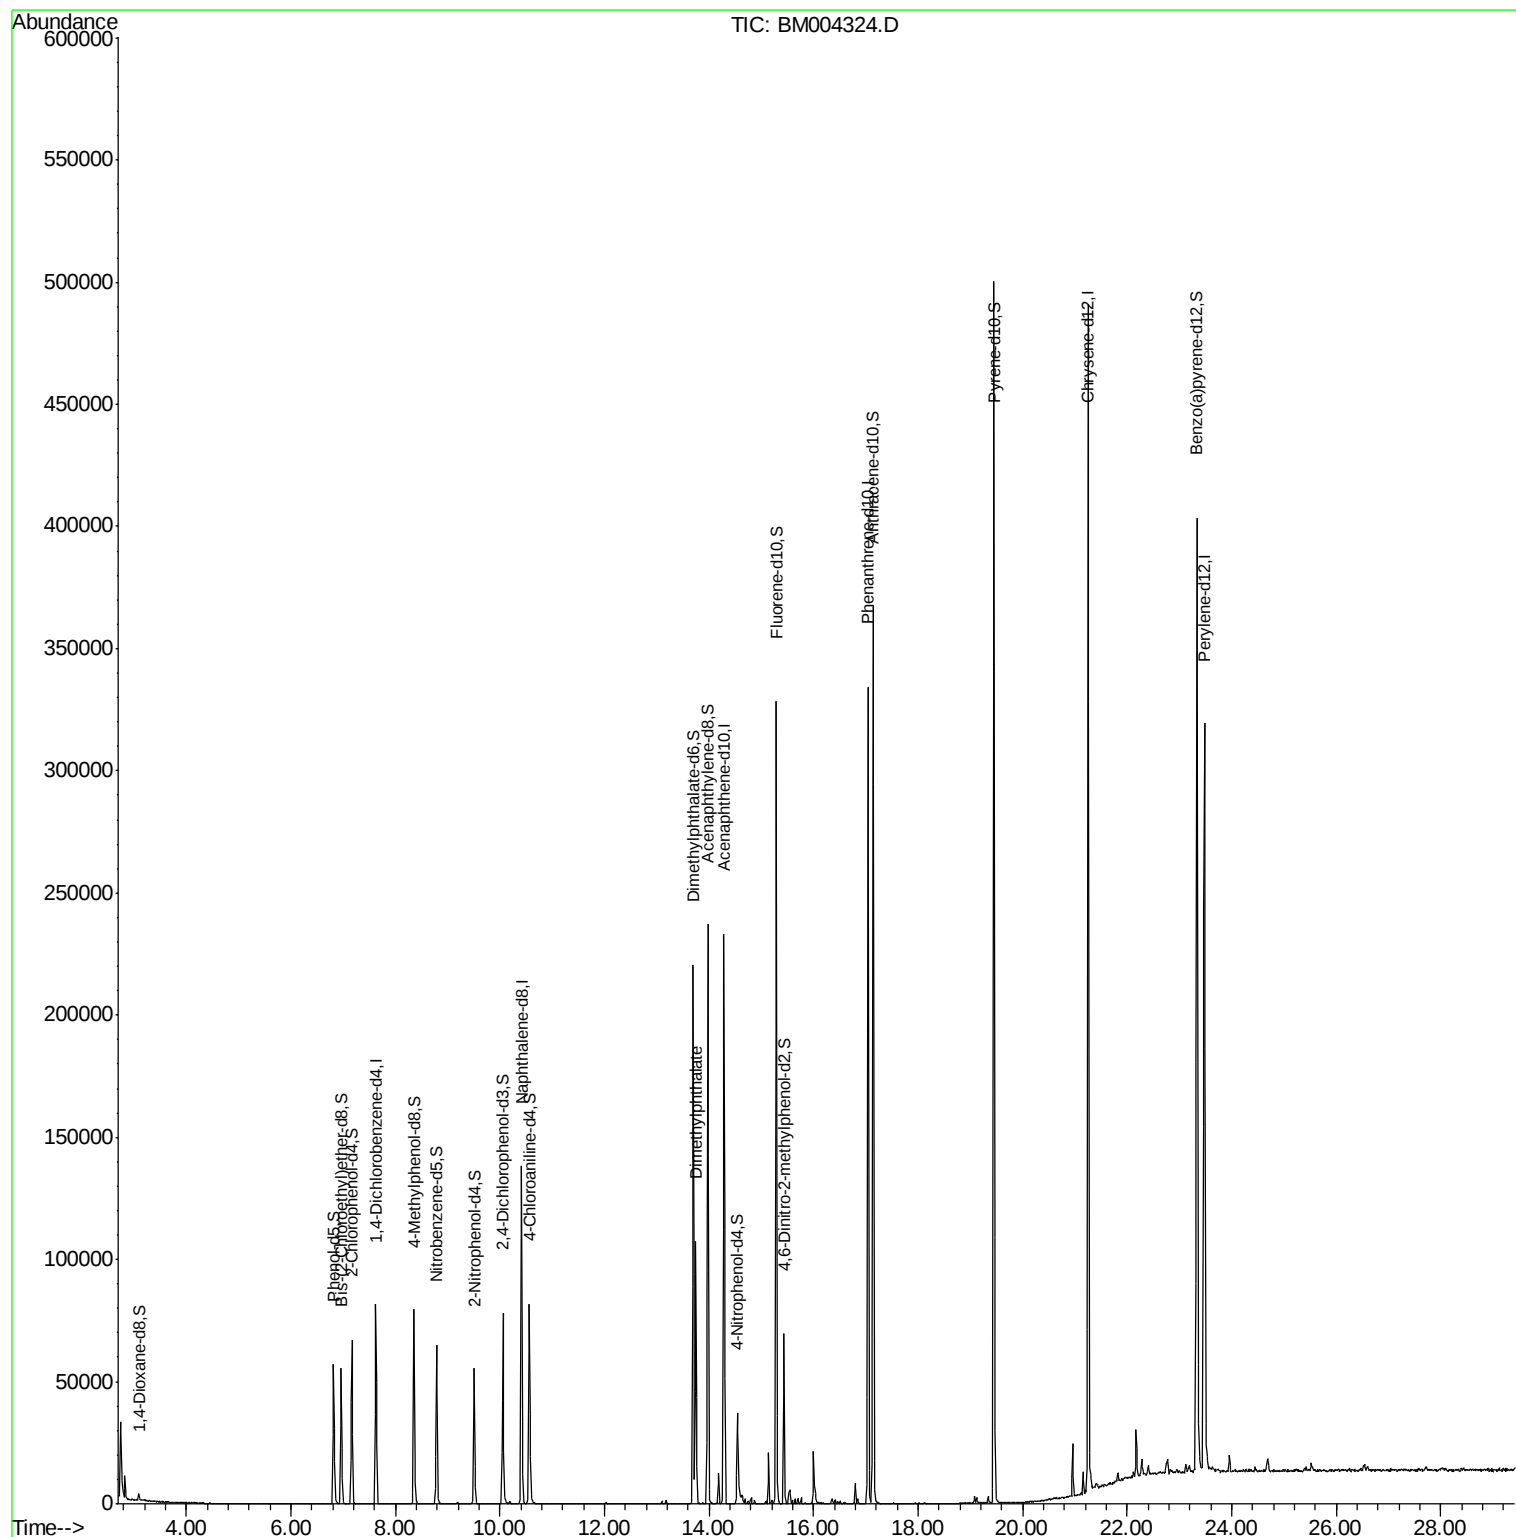

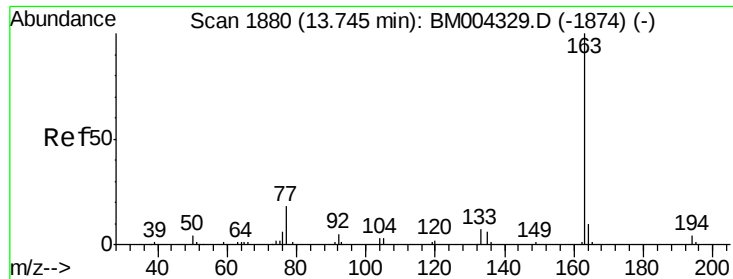

#45
 Dimethylphthalate
 Concen: 10.18 ng/ul
 RT: 13.75 min Scan# 1880
 Delta R.T. 0.00 min
 Lab File: BM004324.D
 Acq: 22 Feb 2016 22:56

Instrument :
 BNA_M
 ClientSampleId :
 0311-S10-0312

Tot Ion:	163	Resp:	73241
Ion Ratio	Lower	Upper	
163	100		
194	4.0	3.2	4.8
164	10.4	7.8	11.8

Manual Integrations
 APPROVED

Sohil
 2/23/2016 5:23:31 PM

