

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022216\
 Data File : BM004325.D
 Acq On : 22 Feb 2016 23:32
 Operator : SJ/UM
 Sample : H1499-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-S36-0003

Manual Integrations
 APPROVED

Sohil
 2/23/2016 5:23:22 PM

Quant Time: Feb 23 00:52:47 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM022216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 23 00:11:03 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	27376	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	130491	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	83377	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	201501	20.00	ng/ul	0.00
78) Chrysene-d12	21.25	240	235901	20.00	ng/ul	0.00
86) Perylene-d12	23.47	264	211400	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.08	96	3240	6.24	ng/uL	0.00
5) Phenol-d5	6.82	99	70335m	30.64	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	39059	33.46	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	62598	31.62	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	64065	31.23	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	32172	32.41	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	37412	33.06	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	63199m	30.90	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	96579	37.88	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	246666	34.50	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	286351	34.21	ng/ul	0.00
52) 4-Nitrophenol-d4	14.53	143	34414	29.94	ng/ul	0.00
58) Fluorene-d10	15.29	176	210379	34.60	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.43	200	33116	26.75	ng/ul	0.00
71) Anthracene-d10	17.14	188	336082	34.04	ng/ul	0.00
79) Pyrene-d10	19.45	212	397950	34.87	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.33	264	390754	35.22	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.74	163	77294	10.37	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM022216\
Data File : BM004325.D
Acq On : 22 Feb 2016 23:32
Operator : SJ/UM
Sample : H1499-08
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
0311-S36-0003

Manual Integrations
APPROVED

Sohil
2/23/2016 5:23:22 PM

Quant Time: Feb 23 00:52:47 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 23 00:11:03 2016
Response via : Initial Calibration

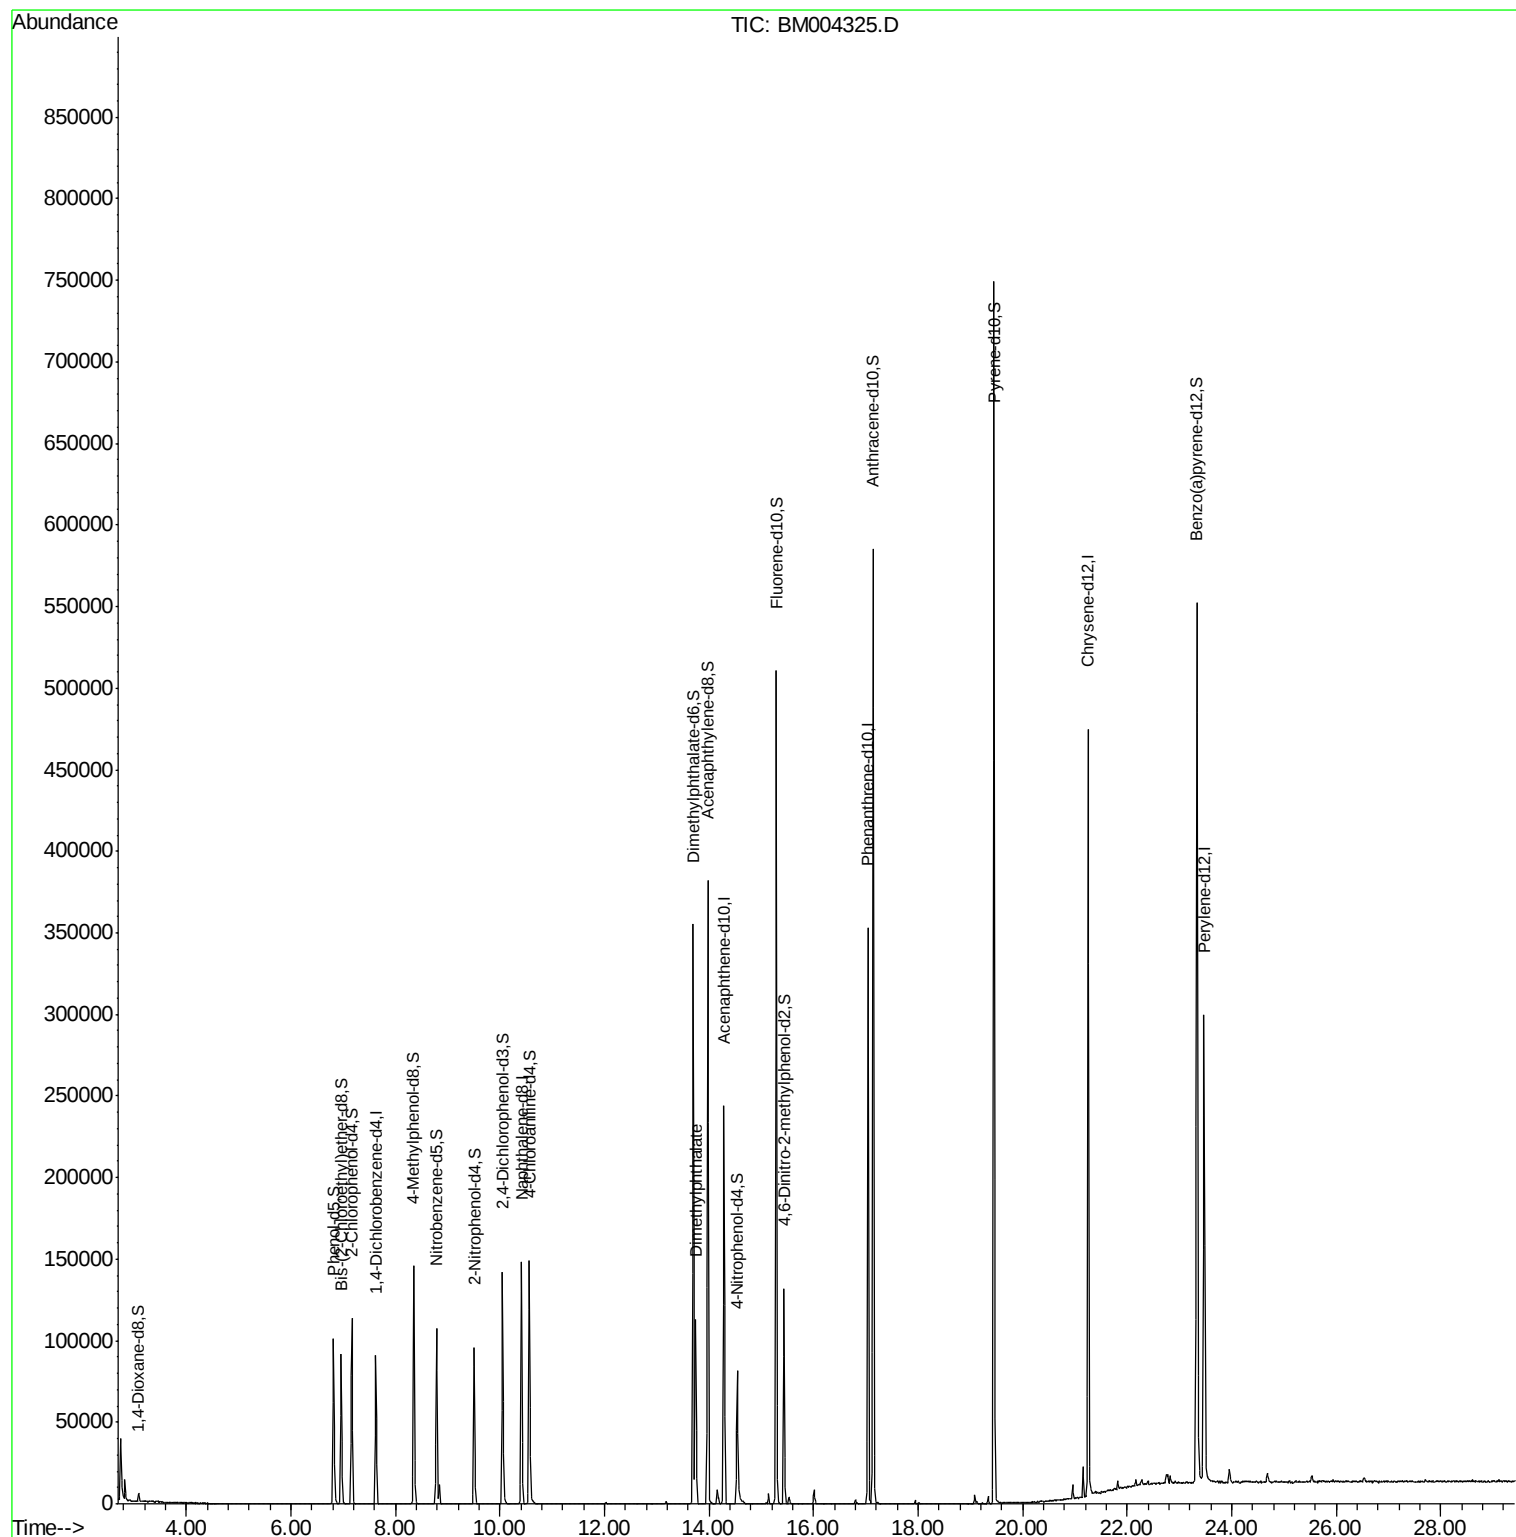

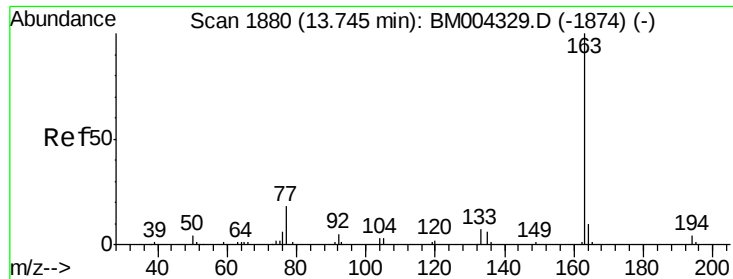


#45
 Dimethylphthalate
 Concen: 10.37 ng/ul
 RT: 13.74 min Scan# 1880
 Delta R.T. -0.00 min
 Lab File: BM004325.D
 Acq: 22 Feb 2016 23:32

Instrument :
 BNA_M
 ClientSampleId :
 0311-S36-0003

Tot Ion	Ratio	Resp	Lower	Upper
163	100	77294		
194	4.0		3.2	4.8
164	10.2		7.8	11.8

Manual Integrations
 APPROVED

Sohil
 2/23/2016 5:23:22 PM

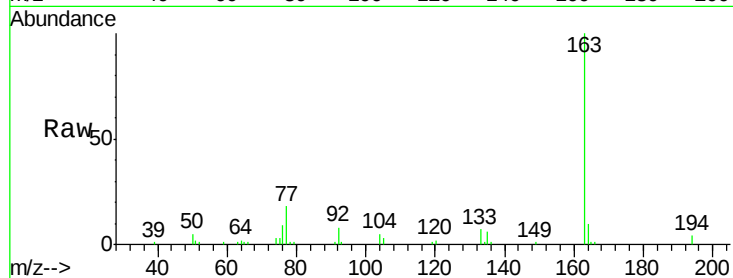

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

