

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022216\
 Data File : BM004332.D
 Acq On : 23 Feb 2016 03:44
 Operator : SJ/UM
 Sample : H1499-16
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-S21-0312

Manual Integrations
 APPROVED

Sohil
 2/23/2016 5:24:27 PM

Quant Time: Feb 23 07:13:43 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM022216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 23 07:03:02 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	30822	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	147925	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	92739	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	215165	20.00	ng/ul	0.00
78) Chrysene-d12	21.24	240	202170	20.00	ng/ul	0.00
86) Perylene-d12	23.47	264	149864	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.09	96	2082	3.56	ng/uL	0.00
5) Phenol-d5	6.82	99	42217m	16.34	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	25965	19.75	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	41156	18.46	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	37710	16.33	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	20462	18.18	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	23243	18.12	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	40770m	17.58	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	57506	19.90	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	156672	19.70	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	187241	20.11	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	12150	9.50	ng/ul	0.00
58) Fluorene-d10	15.29	176	138477	20.47	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.43	200	14924	11.29	ng/ul	0.00
71) Anthracene-d10	17.14	188	215325	20.42	ng/ul	0.00
79) Pyrene-d10	19.44	212	237386	24.27	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.33	264	164628	20.93	ng/ul	0.00

Target Compounds					Ovalue
45) Dimethylphthalate	13.75	163	57128	6.89 ng/ul	100
80) Pyrene	19.47	202	13655	1.03 ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM022216\
Data File : BM004332.D
Acq On : 23 Feb 2016 03:44
Operator : SJ/UM
Sample : H1499-16
Misc :
ALS Vial : 22 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampled :
0311-S21-0312

Manual Integrations
APPROVED

Sohil
2/23/2016 5:24:27 PM

Quant Time: Feb 23 07:13:43 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 23 07:03:02 2016
Response via : Initial Calibration

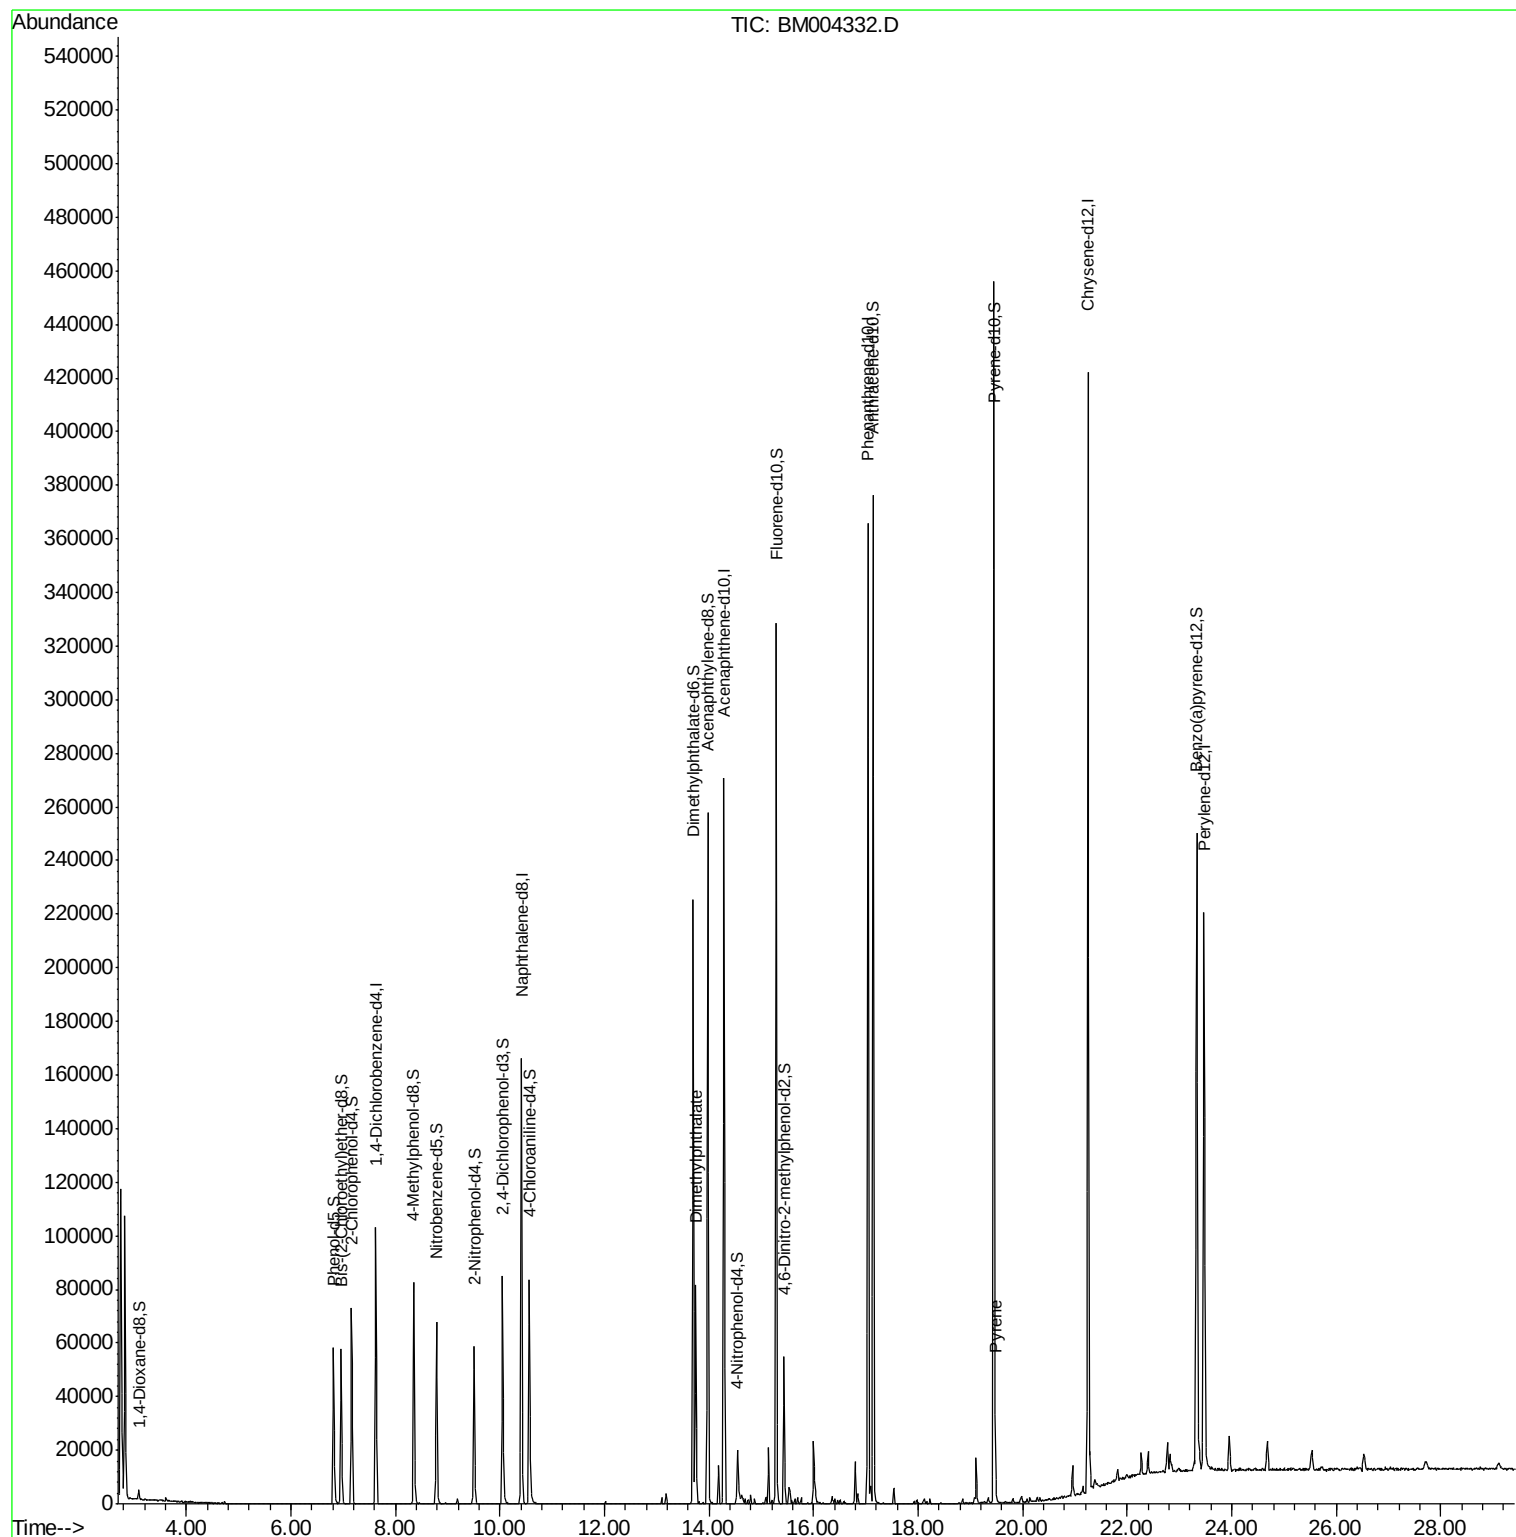

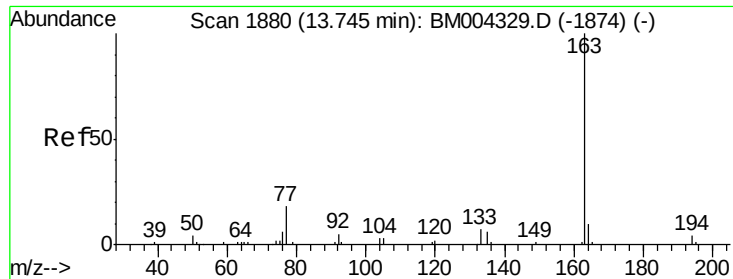

#45

Dimethylphthalate

Concen: 6.89 ng/ul

RT: 13.75 min Scan# 1880

Delta R.T. 0.00 min

Lab File: BM004332.D

Acq: 23 Feb 2016 03:44

Instrument :

BNA_M


ClientSampleId :

0311-S21-0312




Tot Ion:	163	Resp:	57128
Ion Ratio	Lower	Upper	
163	100		
194	4.1	3.2	4.8
164	9.9	7.8	11.8

Manual Integrations
APPROVED

Sohil
2/23/2016 5:24:27 PM

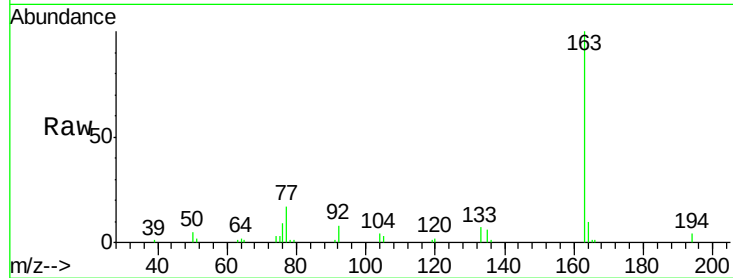

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

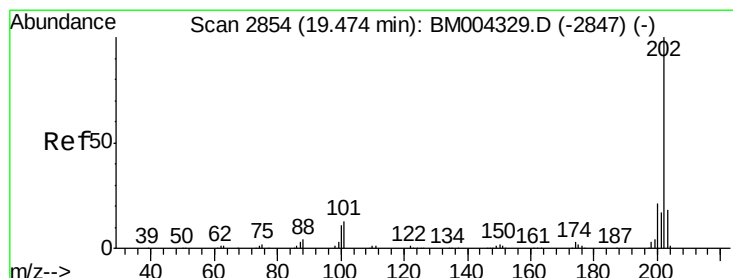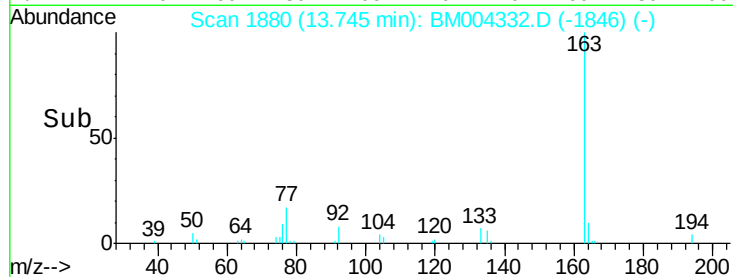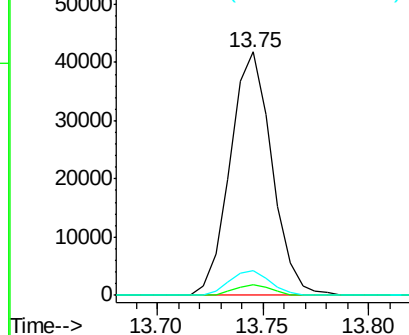

#80

Pyrene

Concen: 1.03 ng/ul

RT: 19.47 min Scan# 2854

Delta R.T. 0.00 min

Lab File: BM004332.D

Acq: 23 Feb 2016 03:44

Tgt Ion:	202	Resp:	13655
Ion Ratio	Lower	Upper	
202	100		
101	11.7	10.2	15.2
100	11.0	8.5	12.7

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

