

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022216\
 Data File : BM004333.D
 Acq On : 23 Feb 2016 04:20
 Operator : SJ/UM
 Sample : H1499-17
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-S22-0003

Manual Integrations
 APPROVED

Sohil
 2/23/2016 5:24:29 PM

Quant Time: Feb 23 07:15:38 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM022216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 23 07:03:02 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	30138	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	145700	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	91922	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	218132	20.00	ng/ul	0.00
78) Chrysene-d12	21.25	240	254874	20.00	ng/ul	0.00
86) Perylene-d12	23.47	264	237115	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.08	96	3569	6.24	ng/uL	0.00
5) Phenol-d5	6.82	99	78443m	31.04	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	44548	34.66	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	71832	32.96	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	72640	32.17	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	36688	33.10	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	43080	34.09	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	73463m	32.16	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	108549	38.13	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	271561	34.45	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	321146	34.80	ng/ul	0.00
52) 4-Nitrophenol-d4	14.53	143	37407	29.52	ng/ul	0.00
58) Fluorene-d10	15.29	176	232860	34.73	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.43	200	37450	27.95	ng/ul	0.00
71) Anthracene-d10	17.14	188	378539	35.42	ng/ul	0.00
79) Pyrene-d10	19.44	212	437194	35.46	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.33	264	445459	35.80	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.74	163	113386	13.79	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM022216\
Data File : BM004333.D
Acq On : 23 Feb 2016 04:20
Operator : SJ/UM
Sample : H1499-17
Misc :
ALS Vial : 23 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
0311-S22-0003

Manual Integrations
APPROVED

Sohil
2/23/2016 5:24:29 PM

Quant Time: Feb 23 07:15:38 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 23 07:03:02 2016
Response via : Initial Calibration

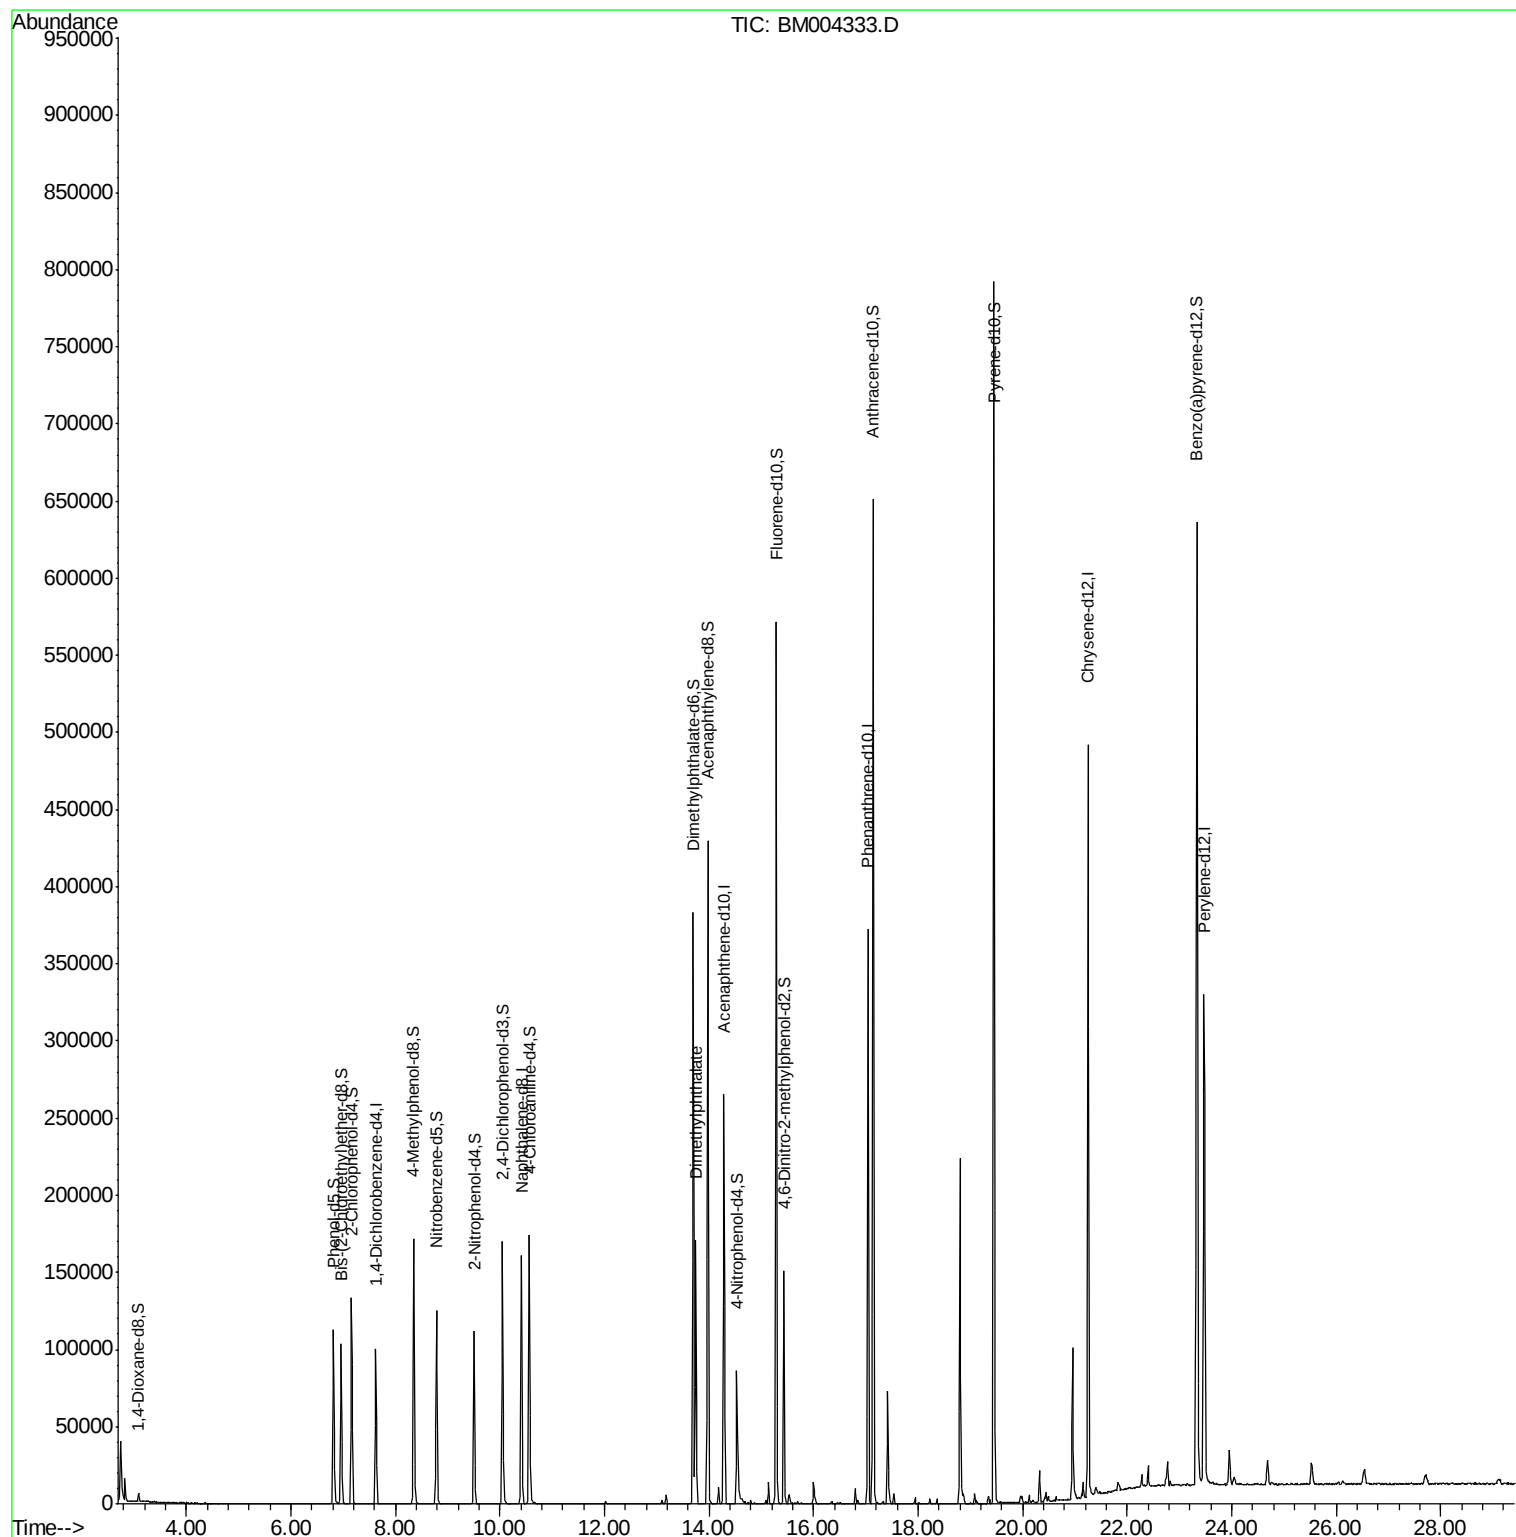

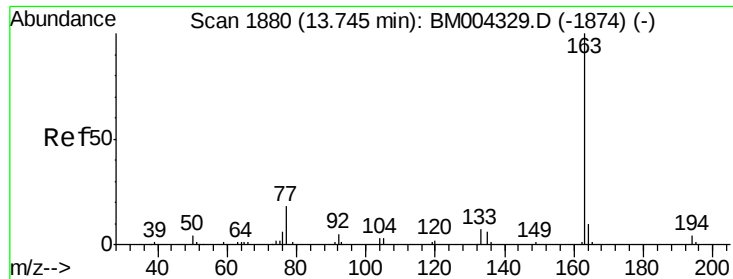

#45
 Dimethylphthalate
 Concen: 13.79 ng/ul
 RT: 13.74 min Scan# 1880
 Delta R.T. -0.00 min
 Lab File: BM004333.D
 Acq: 23 Feb 2016 04:20

Instrument :
 BNA_M
 ClientSampleId :
 0311-S22-0003

Tot Ion:	163	Resp:	113386
Ion Ratio	Lower	Upper	
163	100		
194	4.1	3.2	4.8
164	10.0	7.8	11.8

Manual Integrations
 APPROVED

Sohil
 2/23/2016 5:24:29 PM

