

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022216\
 Data File : BM004324.D
 Acq On : 22 Feb 2016 22:56
 Operator : SJ/UM
 Sample : H1499-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-S10-0312

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.740	5	9	20	rVV	30724	53179	7.37%	0.767%
2	2.822	20	23	30	rVB	9362	12123	1.68%	0.175%
3	3.087	65	68	75	rVB	2559	3408	0.47%	0.049%
4	6.816	697	702	713	rBV	57396	92243	12.78%	1.331%
5	6.963	721	727	736	rBB	55359	83692	11.60%	1.207%
6	7.163	755	761	770	rBB	67338	104808	14.52%	1.512%
7	7.622	834	839	847	rBB	81805	128285	17.78%	1.851%
8	8.351	957	963	974	rBB	79781	131219	18.18%	1.893%
9	8.787	1031	1037	1047	rBB	65107	103177	14.30%	1.488%
10	9.504	1154	1159	1167	rBB	55680	85823	11.89%	1.238%
11	10.051	1246	1252	1268	rBB	78253	137209	19.01%	1.979%
12	10.192	1274	1276	1278	rBB	1288	1155	0.16%	0.017%
13	10.410	1306	1313	1323	rBB	138091	221551	30.70%	3.196%
14	10.557	1333	1338	1358	rBB	81977	148637	20.60%	2.144%
15	12.028	1585	1588	1590	rBB	729	736	0.10%	0.011%
16	13.098	1768	1770	1772	rBB	1215	922	0.13%	0.013%
17	13.180	1781	1784	1786	rBB	1638	1916	0.27%	0.028%
18	13.698	1866	1872	1876	rBV	220796	294405	40.80%	4.247%
19	13.745	1876	1880	1888	rVB	107576	142881	19.80%	2.061%
20	13.974	1913	1919	1933	rBB	237197	345176	47.83%	4.980%
21	14.180	1948	1954	1958	rBB	12385	15247	2.11%	0.220%
22	14.286	1966	1972	1979	rBB2	233345	349093	48.37%	5.036%
23	14.533	2010	2014	2027	rBV	37408	81056	11.23%	1.169%
24	14.627	2027	2030	2036	rVV4	3821	7531	1.04%	0.109%
25	14.680	2036	2039	2042	rVB	2038	1999	0.28%	0.029%
26	14.745	2047	2050	2051	rBB	1223	1207	0.17%	0.017%
27	14.804	2057	2060	2062	rBB	2779	3166	0.44%	0.046%
28	14.874	2069	2072	2074	rBB	1345	1117	0.15%	0.016%
29	15.086	2106	2108	2112	rBB	1064	1148	0.16%	0.017%
30	15.139	2112	2117	2121	rBB	21195	25086	3.48%	0.362%
31	15.198	2124	2127	2130	rBB2	1476	1593	0.22%	0.023%
32	15.286	2136	2142	2152	rBB	328689	468307	64.89%	6.756%
33	15.427	2162	2166	2176	rBB	69878	96174	13.33%	1.387%
34	15.527	2179	2183	2185	rBV	5302	8467	1.17%	0.122%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022216\
 Data File : BM004324.D
 Acq On : 22 Feb 2016 22:56
 Operator : SJ/UM
 Sample : H1499-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-S10-0312

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
 Title : SVOA CALIBRATION

35	15.586	2190	2193	2195	rBB	1559	1343	0.19%	0.019%
36	15.639	2200	2202	2204	rBB	1892	1701	0.24%	0.025%
37	15.698	2208	2212	2214	rBB	2197	2515	0.35%	0.036%
38	15.763	2219	2223	2225	rBB	2543	2188	0.30%	0.032%
39	15.998	2259	2263	2274	rBV	21527	36347	5.04%	0.524%
40	16.345	2318	2322	2330	rBB	2174	4225	0.59%	0.061%
41	16.404	2330	2332	2336	rBB	1560	1538	0.21%	0.022%
42	16.463	2340	2342	2343	rBB	1057	742	0.10%	0.011%
43	16.510	2348	2350	2352	rBB	1174	936	0.13%	0.014%
44	16.792	2394	2398	2402	rVB2	8326	9434	1.31%	0.136%
45	16.839	2402	2406	2410	rBB2	2280	3202	0.44%	0.046%
46	17.039	2434	2440	2446	rBV	334432	454721	63.01%	6.560%
47	17.139	2451	2457	2471	rVV	367623	527072	73.04%	7.604%
48	19.080	2783	2787	2790	rBV	2667	3163	0.44%	0.046%
49	19.115	2790	2793	2797	rVB	2322	2581	0.36%	0.037%
50	19.333	2827	2830	2834	rBV	2576	2786	0.39%	0.040%
51	19.445	2843	2849	2859	rBV	499827	683825	94.76%	9.865%
52	20.492	3022	3027	3029	rBV2	456	859	0.12%	0.012%
53	20.603	3044	3046	3049	rVV2	826	781	0.11%	0.011%
54	20.951	3101	3105	3112	rBV	21542	27139	3.76%	0.392%
55	21.156	3137	3140	3143	rVB	8548	8311	1.15%	0.120%
56	21.250	3150	3156	3169	rBV	485971	626281	86.78%	9.035%
57	21.398	3177	3181	3182	rBV3	1852	2374	0.33%	0.034%
58	21.815	3250	3252	3256	rVB2	3355	3591	0.50%	0.052%
59	22.168	3308	3312	3317	rBV	19260	25216	3.49%	0.364%
60	22.274	3326	3330	3336	rBV2	6628	11081	1.54%	0.160%
61	22.744	3406	3410	3411	rBV2	3777	5147	0.71%	0.074%
62	23.333	3502	3510	3523	rBV	389866	721663	100.00%	10.411%
63	23.474	3526	3534	3548	rVB	305426	596374	82.64%	8.603%
64	23.950	3611	3615	3620	rBV2	6637	10919	1.51%	0.158%


Sum of corrected areas: 6931791

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022216\
Data File : BM004324.D
Acq On : 22 Feb 2016 22:56
Operator : SJ/UM
Sample : H1499-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0311-S10-0312

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

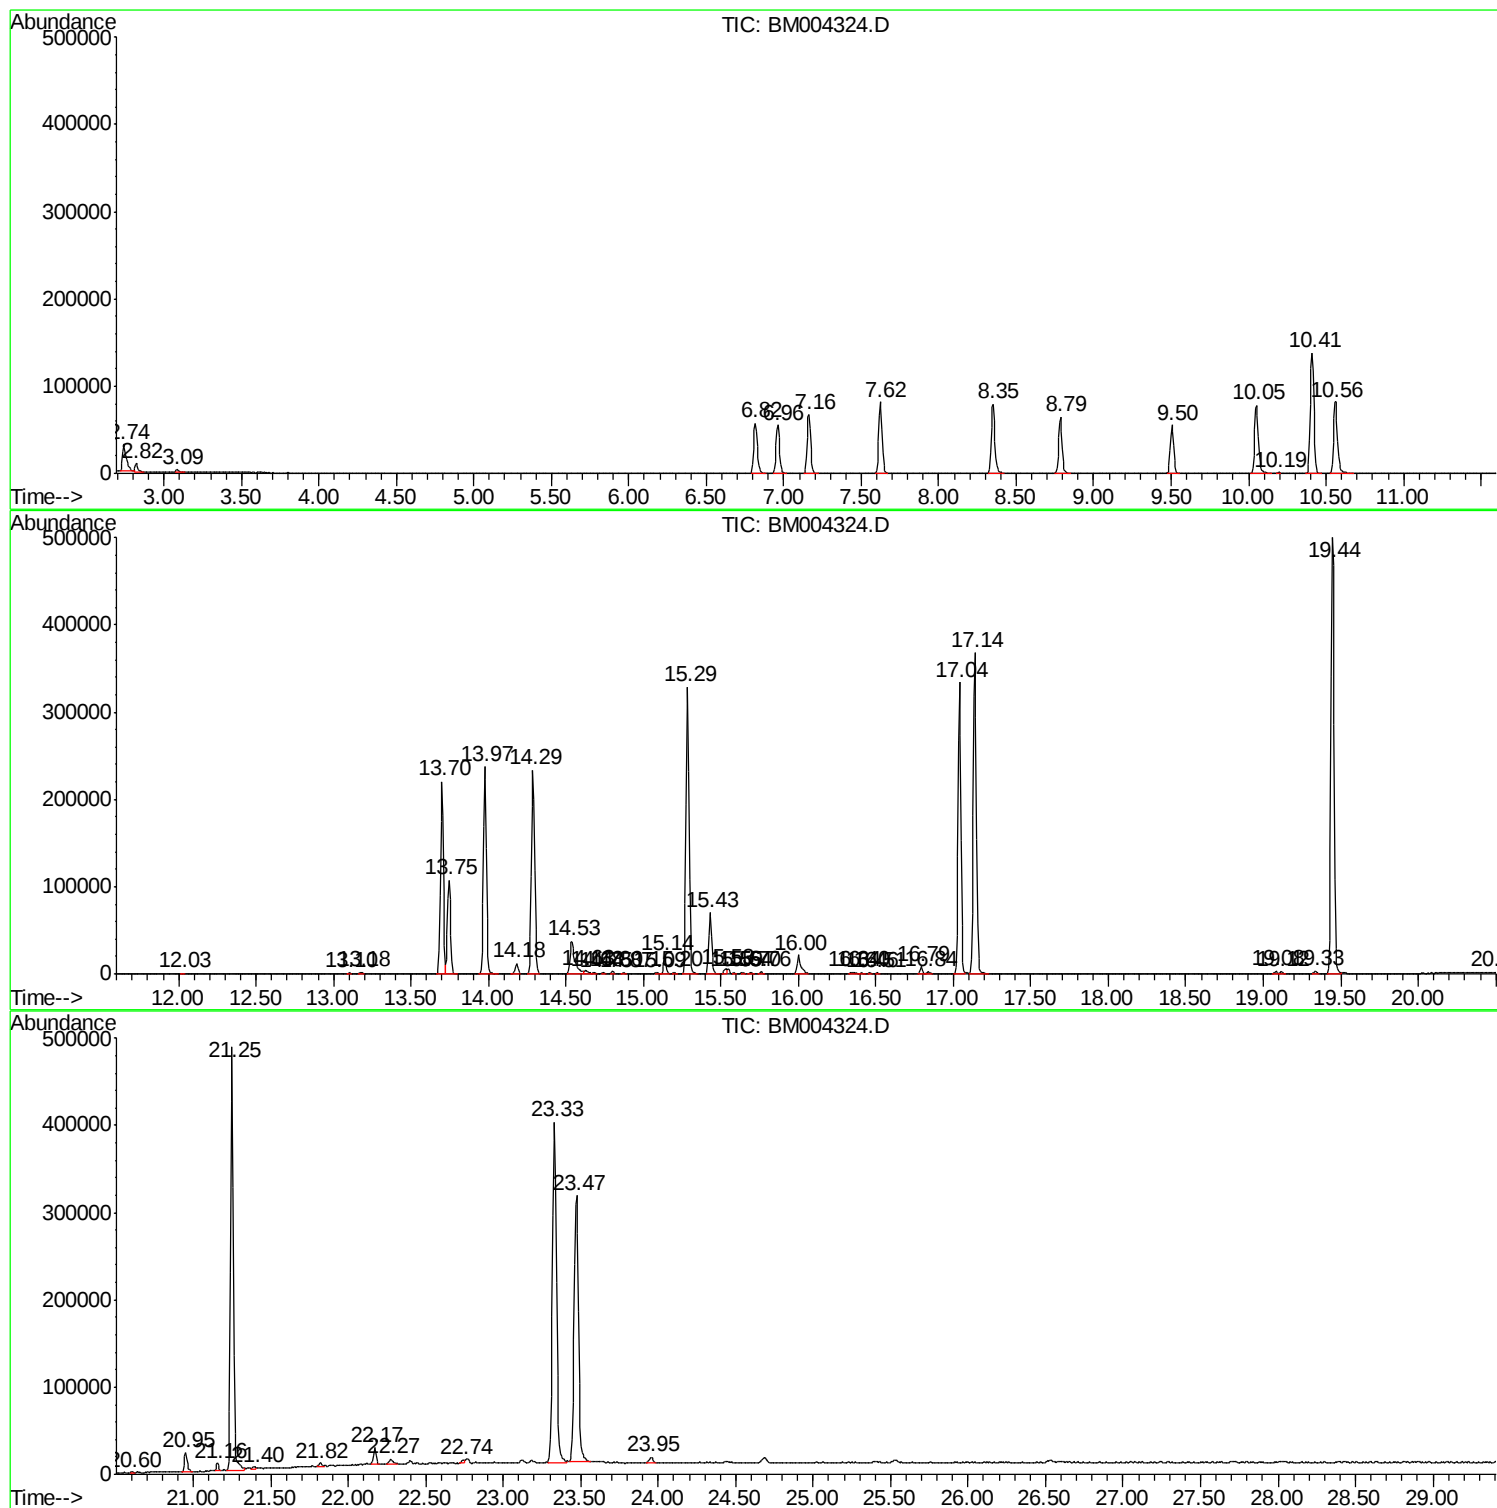

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022216\
Data File : BM004324.D
Acq On : 22 Feb 2016 22:56
Operator : SJ/UM
Sample : H1499-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0311-S10-0312

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022216\
Data File : BM004324.D
Acq On : 22 Feb 2016 22:56
Operator : SJ/UM
Sample : H1499-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0311-S10-0312

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc