


Data Path : Z:\HPCHEM1\BNA M\DATA\BM022216\
Data File : BM004309.D
Acq On : 22 Feb 2016 12:21
Operator : SJ/UM
Sample : DFTPP53
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP53

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Title : SVOA CALIBRATION
Last Update : Tue Feb 23 07:03:02 2016

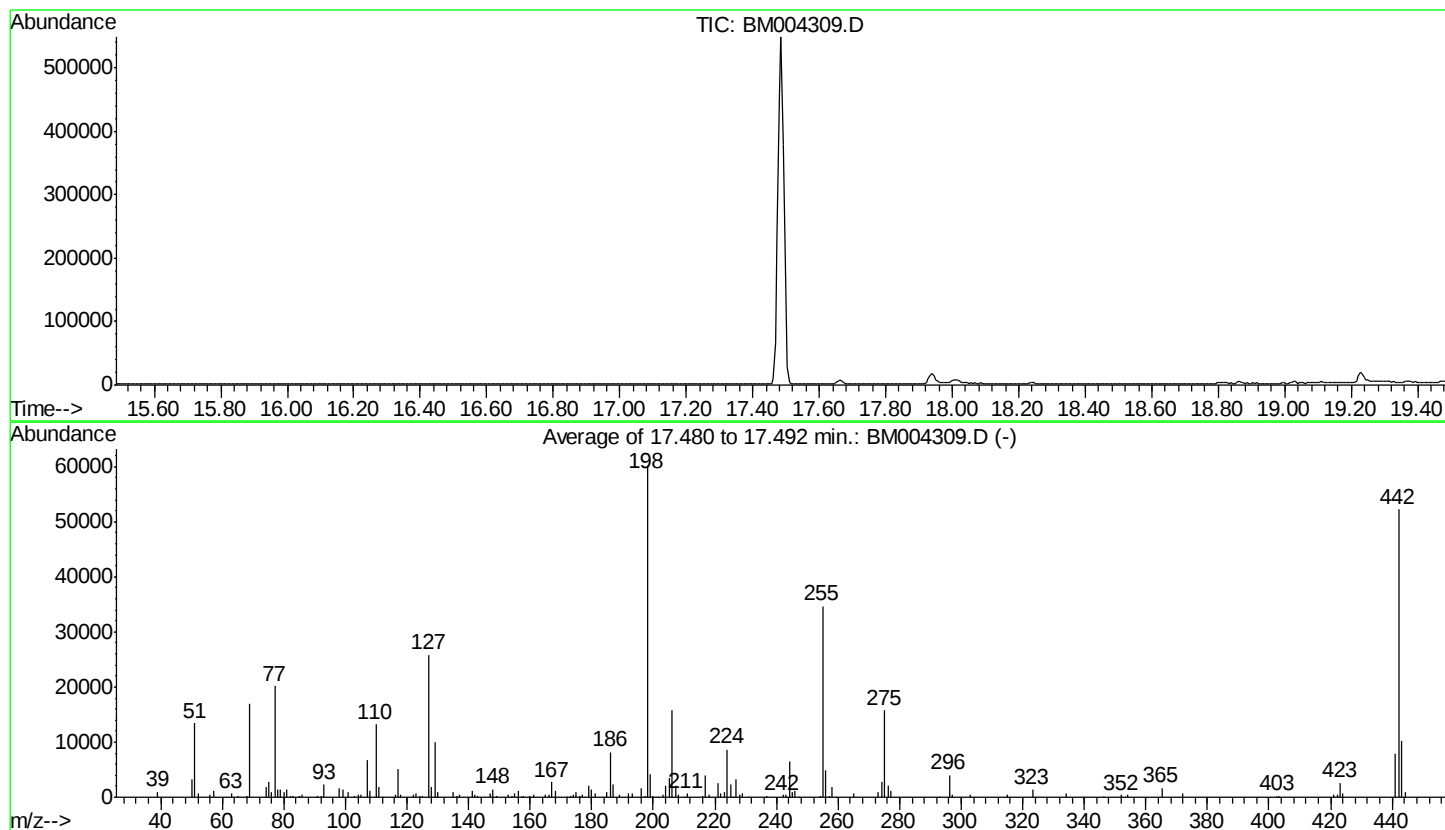

AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.3	13427	PASS
68	69	0.00	2	1.5	260	PASS
69	198	0.00	100	28.2	16997	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.0	25898	PASS
197	198	0.00	2	0.5	281	PASS
198	198	100	100	100.0	60168	PASS
199	198	5	9	6.8	4079	PASS
275	198	10	60	26.2	15754	PASS
365	198	1	100	2.8	1689	PASS
441	443	0.01	100	77.7	7946	PASS
442	198	50	100	86.7	52154	PASS
443	442	15	24	19.6	10220	PASS

m/z	Abundance
39.10	1194.0
43.10	783.0
45.00	535.0
50.10	3667.0
51.10	15435.0
52.10	776.0
56.00	549.0
57.00	1134.0
60.00	457.0
63.00	702.0
65.00	355.0
68.10	390.0
69.00	19248.0
74.00	2017.0
75.00	3090.0
76.10	1110.0
77.10	22528.0
78.10	1556.0
79.00	1542.0
80.00	1179.0
81.00	1680.0
82.00	430.0
83.00	422.0
85.00	377.0
86.00	472.0
91.00	390.0
92.00	394.0
93.00	2629.0
98.00	1933.0
99.00	1673.0
101.00	1008.0
103.00	371.0
104.00	639.0
105.00	651.0
107.00	7512.0
108.00	1205.0
110.00	14420.0
111.00	2097.0
112.00	308.0
116.10	391.0
117.00	5443.0
118.00	415.0
122.00	580.0
123.00	798.0
123.90	319.0
125.00	358.0
127.10	27856.0
128.10	2112.0
129.00	10623.0
130.00	915.0
135.00	911.0
136.00	393.0
137.00	470.0
141.00	1391.0
142.00	522.0
143.00	307.0
147.00	745.0
148.00	1385.0
149.10	368.0
153.00	448.0
154.00	326.0
155.00	723.0
156.00	1202.0
157.00	304.0
158.00	306.0
160.00	476.0
161.00	553.0
165.00	534.0
166.00	440.0
167.00	2667.0
168.00	1343.0
172.00	305.0
173.00	321.0
174.00	568.0
175.00	1079.0
176.10	367.0
177.00	604.0
179.00	2141.0
180.10	1457.0
181.00	742.0
185.00	1056.0
186.10	8402.0
187.10	2379.0
189.00	495.0
192.00	614.0
193.10	817.0
196.10	1655.0
198.00	60736.0
199.00	4297.0
203.00	352.0
204.10	2180.0
205.10	3669.0

Instrument :
BNA_M
ClientSampleId :
DFTPP53

206.10	15703.0
207.10	2149.0
208.00	537.0
211.00	576.0
216.00	331.0
217.00	4039.0
218.10	522.0
221.10	2458.0
221.90	624.0
223.10	867.0
224.10	8435.0
225.10	2344.0
227.00	3172.0
228.00	395.0
229.00	671.0
237.00	329.0
242.10	426.0
243.00	470.0
244.10	6410.0
245.10	848.0
246.00	1274.0
255.10	33192.0
256.10	4800.0
257.00	424.0
258.10	1775.0
265.00	721.0
273.10	969.0
274.10	2510.0
275.10	14674.0
276.10	1921.0
277.00	1242.0
296.10	3610.0
297.00	494.0
303.10	450.0
315.10	385.0
323.10	1218.0
334.10	673.0
352.00	354.0
354.10	442.0
365.10	1457.0
372.10	618.0
421.10	302.0
422.10	310.0
423.10	2128.0
424.10	581.0
441.10	6340.0
442.20	40776.0
443.10	8166.0
444.10	760.0

Instrument :
BNA_M
ClientSampleId :
DFTPP53

m/z	Abundance
39.10	1149.0
43.00	889.0
45.00	543.0
50.10	3679.0
51.10	15381.0
52.00	823.0
56.00	476.0
57.00	1334.0
60.10	473.0
63.00	726.0
65.00	421.0
68.10	391.0
69.00	19712.0
74.10	2026.0
75.00	3093.0
76.10	1110.0
77.10	23552.0
78.10	1641.0
79.00	1545.0
80.00	1162.0
81.00	1649.0
82.00	378.0
83.10	441.0
85.00	331.0
86.00	486.0
91.00	387.0
92.00	425.0
93.00	2713.0
98.00	2008.0
99.00	1700.0
101.00	1100.0
103.00	384.0
104.00	684.0
105.00	621.0
107.00	7879.0
108.10	1229.0
110.00	15337.0
111.00	2322.0
116.00	400.0
117.00	5850.0
118.00	470.0
122.00	596.0
123.00	840.0
124.00	427.0
125.00	351.0
127.10	30264.0
128.00	2348.0
129.00	11589.0
130.00	1170.0
135.00	967.0
136.00	404.0
137.00	563.0
141.00	1467.0
142.00	545.0
143.00	338.0
147.00	793.0
148.00	1739.0
149.00	363.0
153.00	480.0
154.00	378.0
155.10	915.0
156.00	1348.0
158.00	362.0
160.00	524.0
161.10	657.0
165.00	566.0
166.00	503.0
167.10	3249.0
168.00	1507.0
173.10	328.0
174.00	681.0
175.10	1218.0
176.00	314.0
177.00	678.0
179.00	2377.0
180.10	1689.0
181.00	740.0
185.00	1214.0
186.10	9686.0
187.10	2791.0
189.00	563.0
192.10	758.0
193.00	828.0
196.10	2017.0
197.10	479.0
198.00	71376.0
199.00	4752.0
200.00	384.0
201.50	334.0
203.00	458.0
204.10	2434.0
205.10	4024.0

Instrument :
BNA_M
ClientSampleId :
DFTPP53

206.10	18464.0
207.10	2637.0
208.00	567.0
210.20	305.0
211.00	740.0
216.00	389.0
217.00	4579.0
218.00	603.0
221.10	2997.0
221.80	742.0
223.00	1061.0
224.10	10304.0
225.10	2624.0
226.10	302.0
227.00	4015.0
228.10	607.0
229.00	801.0
231.00	319.0
237.00	379.0
242.00	550.0
243.10	494.0
244.10	7485.0
245.10	1000.0
246.00	1479.0
247.00	331.0
254.20	394.0
255.10	41136.0
256.10	5955.0
257.00	483.0
258.00	2085.0
259.10	323.0
265.00	890.0
273.10	1268.0
274.10	3239.0
275.10	18632.0
276.10	2351.0
277.10	1426.0
293.10	314.0
296.10	4664.0
297.00	656.0
303.10	544.0
315.00	506.0
323.10	1563.0
324.10	302.0
334.10	926.0
346.00	322.0
352.10	438.0
353.10	336.0
354.10	467.0
365.10	2018.0
372.10	838.0
402.10	321.0
403.10	475.0
421.10	468.0
422.10	414.0
423.10	2993.0
424.10	733.0
441.20	9278.0
442.20	62680.0
443.10	12057.0
444.10	1147.0

Instrument :
BNA_M
ClientSampleId :
DFTPP53

m/z	Abundance
39.10	661.0
43.10	792.0
45.00	635.0
50.00	2291.0
51.10	9466.0
52.10	509.0
56.00	354.0
57.00	740.0
60.00	439.0
63.10	438.0
69.00	12033.0
74.00	1265.0
75.00	1993.0
76.10	629.0
77.10	14253.0
78.10	899.0
79.00	1051.0
80.00	763.0
81.00	1044.0
86.00	341.0
93.00	1615.0
98.00	1300.0
99.00	1031.0
101.00	704.0
104.00	439.0
105.00	405.0
107.00	5052.0
108.00	753.0
110.00	9698.0
111.00	1438.0
116.00	317.0
117.00	3850.0
118.00	339.0
122.00	342.0
123.00	555.0
127.10	19576.0
128.00	1478.0
129.00	7510.0
130.00	669.0
135.00	671.0
137.00	352.0
141.00	985.0
142.00	324.0
147.00	574.0
148.00	1089.0
152.90	384.0
155.10	561.0
156.10	908.0
161.00	525.0
165.00	426.0
166.00	308.0
167.00	2244.0
168.00	918.0
174.00	470.0
175.10	858.0
177.00	385.0
179.00	1576.0
180.00	1175.0
181.00	548.0
185.00	743.0
186.10	6643.0
187.00	1921.0
189.00	448.0
192.00	539.0
193.00	629.0
196.00	1455.0
197.10	365.0
198.00	48392.0
199.00	3188.0
203.00	330.0
204.10	1677.0
205.10	2842.0
206.10	13117.0
207.10	1755.0
208.10	403.0
211.00	496.0
217.00	3340.0
218.00	400.0
221.10	2273.0
221.80	464.0
223.00	734.0
224.10	7084.0
225.10	1911.0
227.00	2804.0
228.00	380.0
229.10	731.0
242.00	366.0
243.10	363.0
244.10	5605.0
245.10	699.0
246.10	1035.0
255.10	29768.0

Instrument :
BNA_M
ClientSampleId :
DFTPP53

256.10	4245.0
258.10	1515.0
265.00	559.0
273.00	817.0
274.10	2400.0
275.10	13956.0
276.10	1790.0
277.00	1139.0
296.10	3594.0
297.10	499.0
303.00	449.0
315.00	422.0
323.10	1211.0
334.10	802.0
352.10	382.0
354.10	468.0
365.10	1593.0
372.10	689.0
403.10	435.0
421.10	328.0
422.10	397.0
423.10	2754.0
424.10	557.0
441.10	8222.0
442.20	53008.0
443.20	10439.0
444.10	899.0

Instrument :
BNA_M
ClientSampleId :
DFTPP53

Scan 2510 (17.451 min): BM004309.D
DFTPP53

m/z	Abundance
43.00	867.0
44.00	312.0
45.00	669.0
60.00	470.0

Instrument :
BNA_M
ClientSampleId :
DFTPP53