


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022221\
Data File : BM028864.D
Acq On : 22 Feb 2021 14:20
Operator : CG/JU
Sample : PB134705BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK05

Manual Integrations
APPROVED

mohammad
2/23/2021 3:44:48 PM

Quant Time: Feb 22 15:03:40 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 22 11:00:59 2021
Response via : Initial Calibration

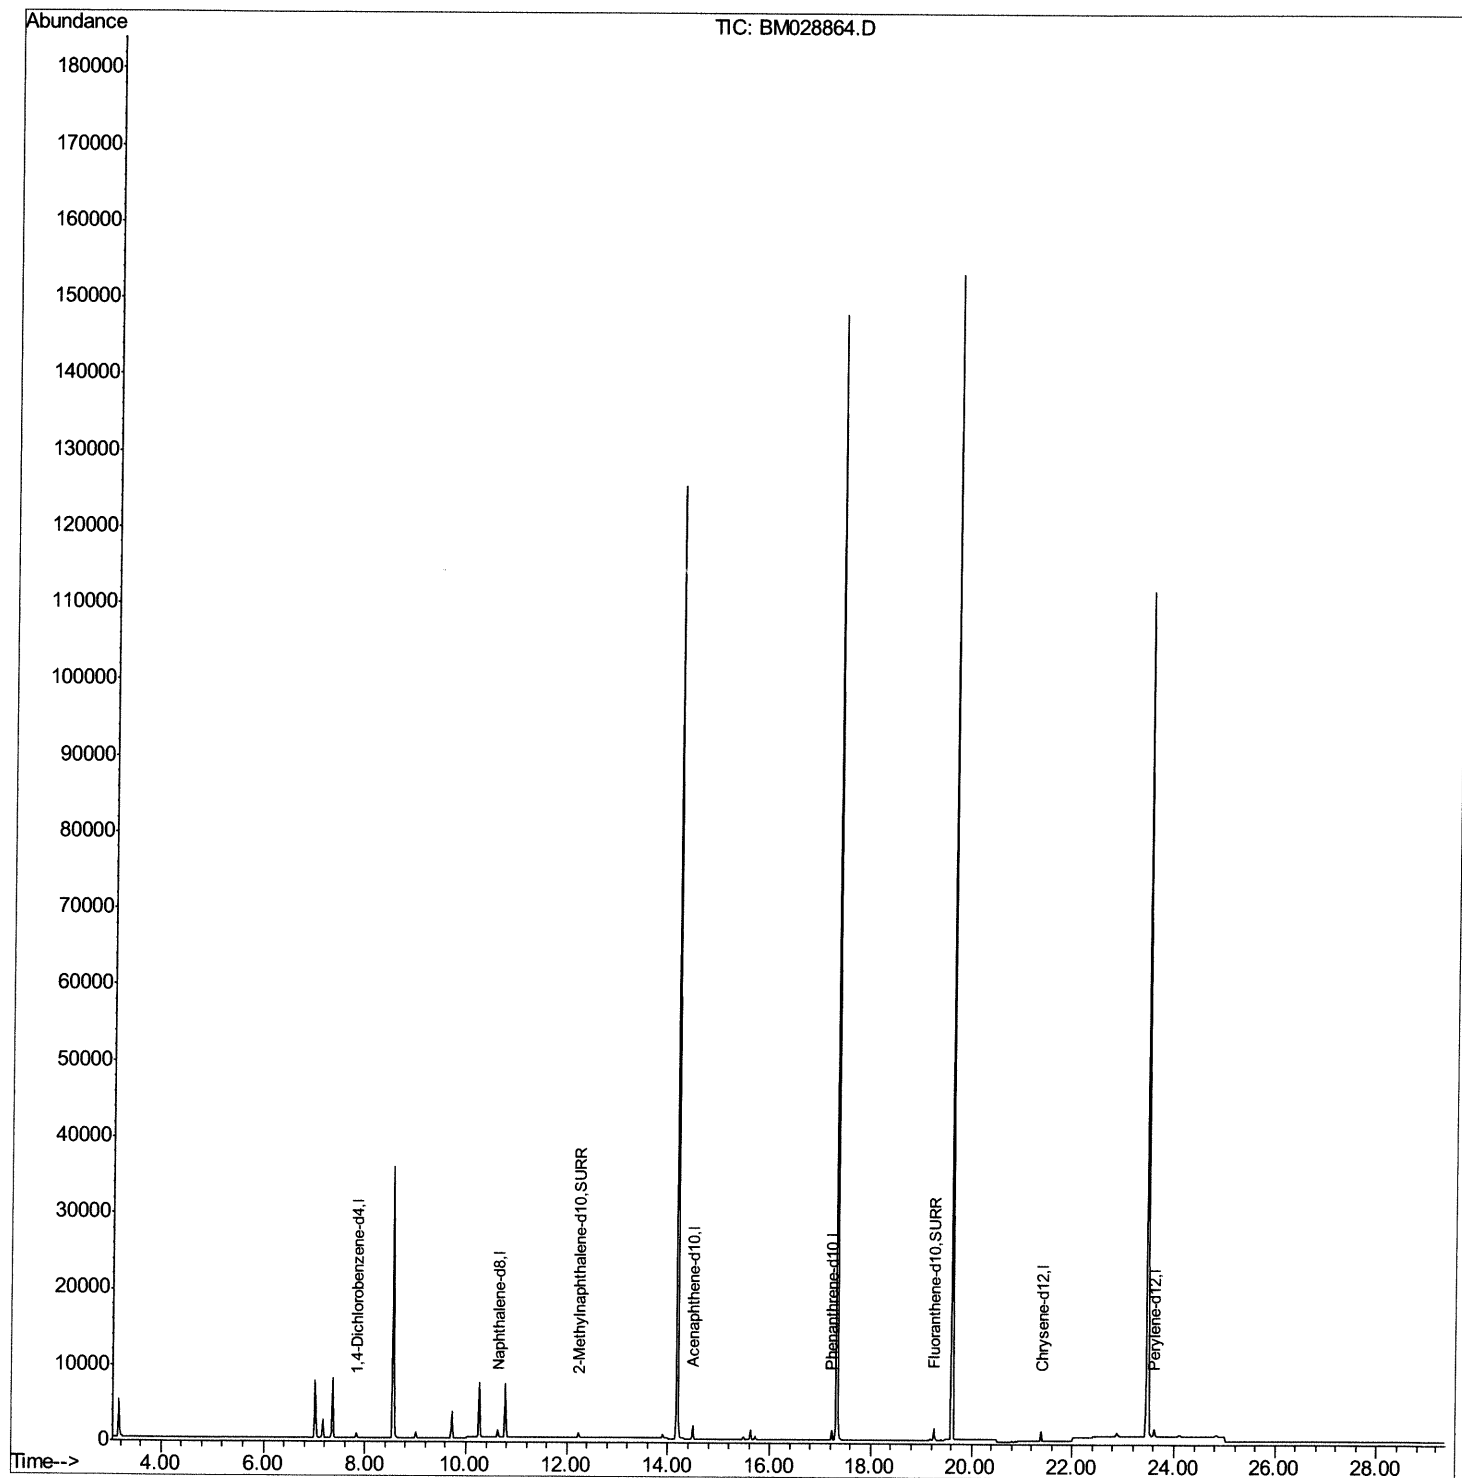

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022221\
 Data File : BM028864.D
 Acq On : 22 Feb 2021 14:20
 Operator : CG/JU
 Sample : PB134705BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 SBLK05

Manual Integrations
APPROVED

mohammad
 2/23/2021 3:44:48 PM

Quant Time: Feb 22 15:02:28 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 22 11:00:59 2021
 Response via : Initial Calibration

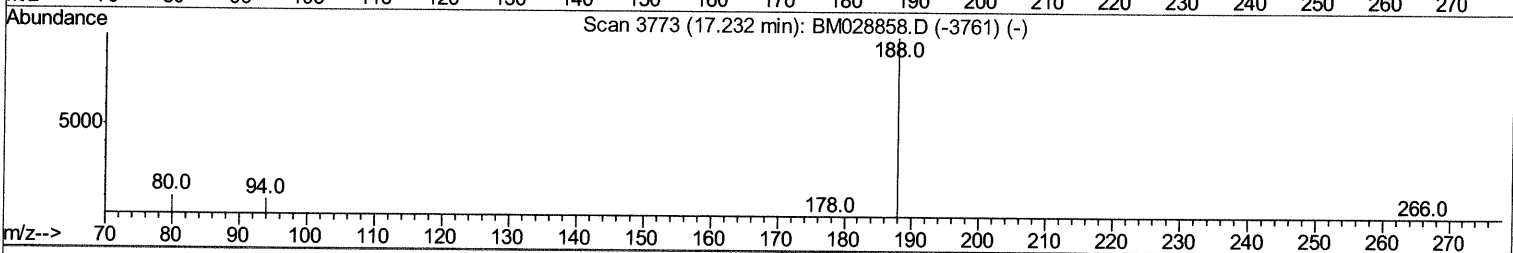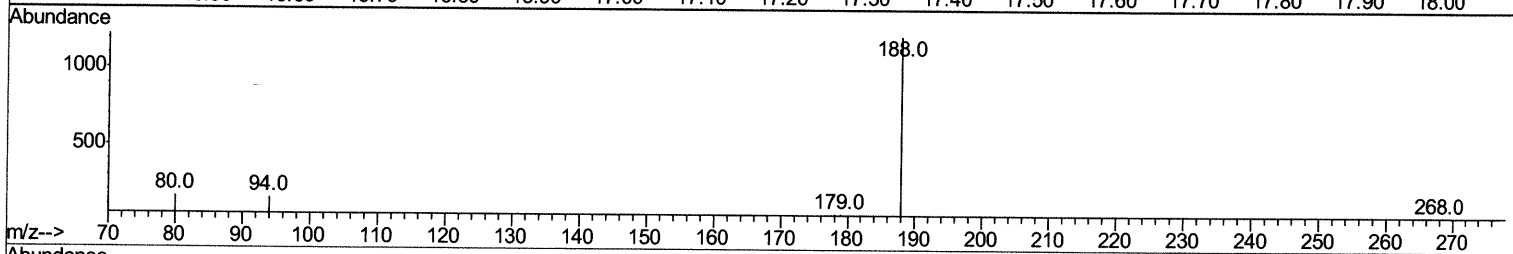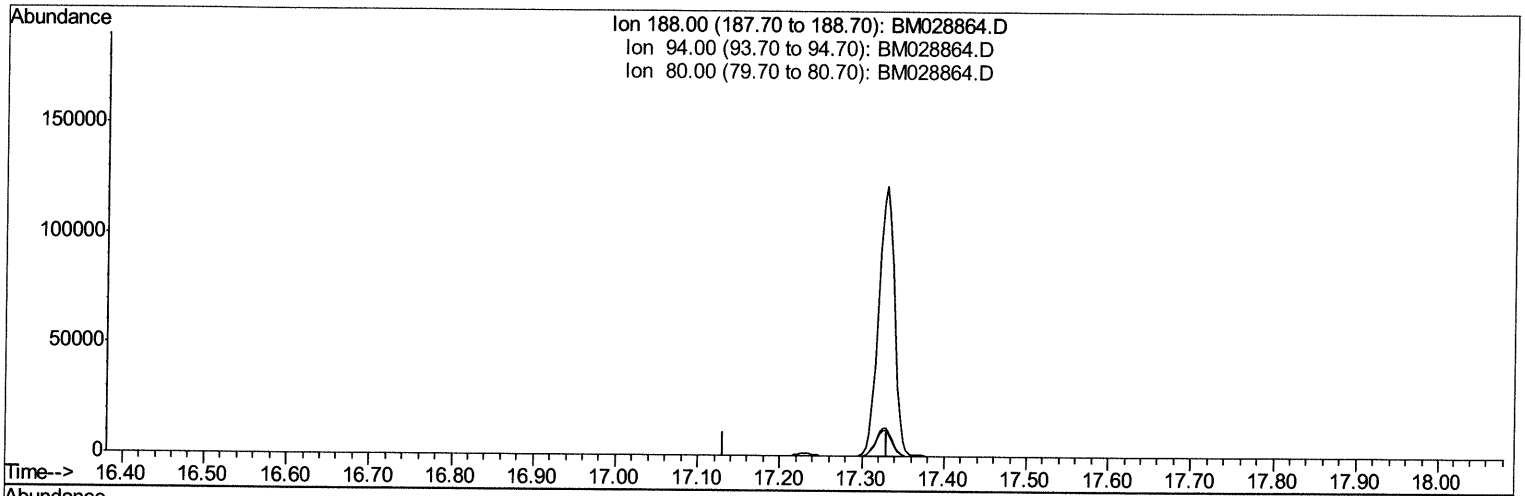

TIC: BM028864.D

(10) Phenanthrene-d10 (I)

17.232min (-17.232) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	13.50	0.00#
80.00	14.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022221\
 Data File : BM028864.D
 Acq On : 22 Feb 2021 14:20
 Operator : CG/JU
 Sample : PB134705BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 SBLK05

Manual Integrations
APPROVED

mohammad
 2/23/2021 3:44:48 PM

Quant Time: Feb 22 15:02:28 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 22 11:00:59 2021
 Response via : Initial Calibration

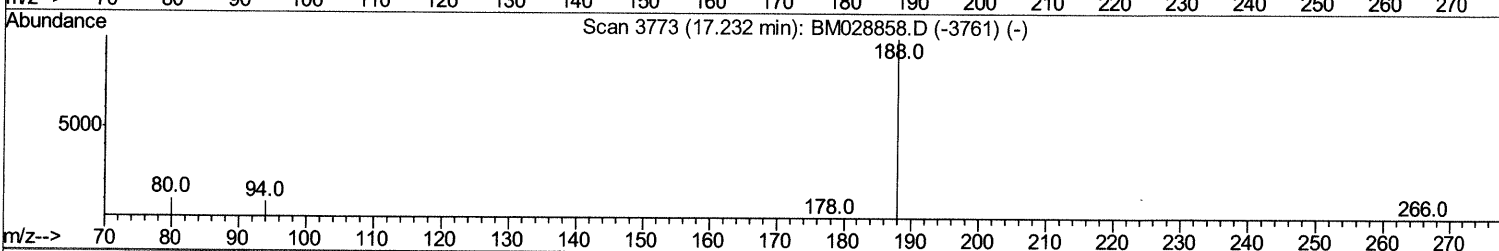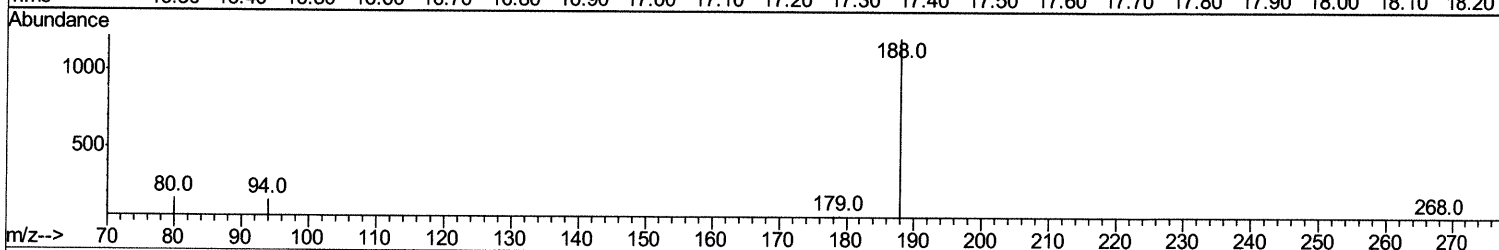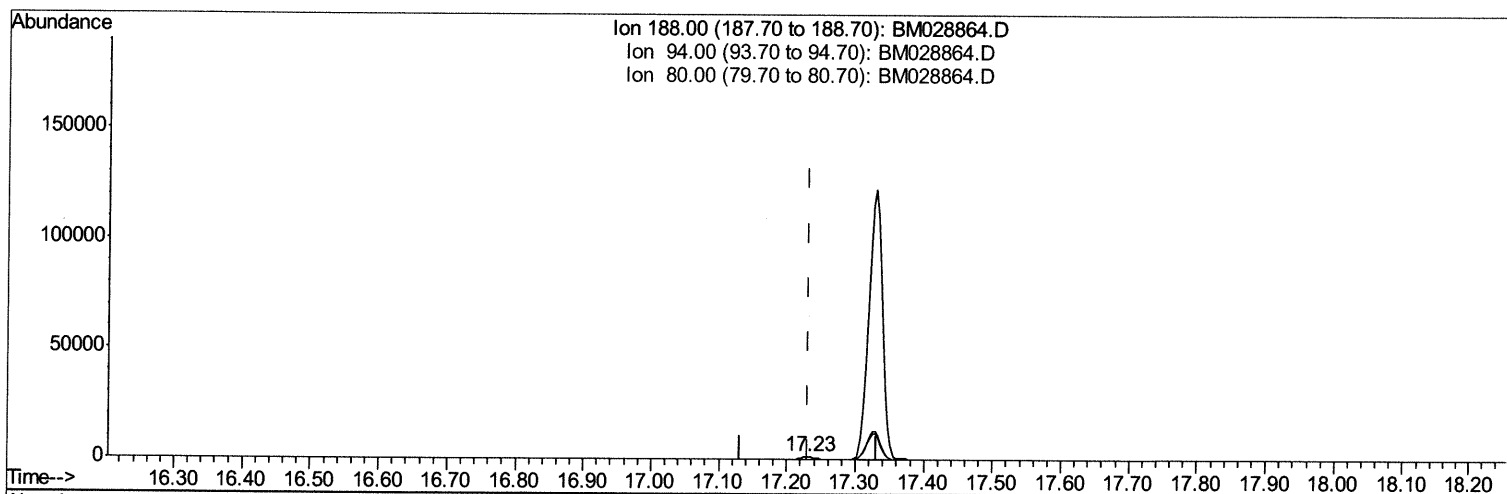

TIC: BM028864.D

(10) Phenanthrene-d10 (I)

17.232min (-0.000) 0.40ng/ul m 02/24/21JU

response 1741

Ion	Exp%	Act%
188.00	100	100
94.00	13.50	12.46
80.00	14.00	13.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022221\
 Data File : BM028864.D
 Acq On : 22 Feb 2021 14:20
 Operator : CG/JU
 Sample : PB134705BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK05

Manual Integrations
 APPROVED

mohammad
 2/23/2021 3:44:48 PM

Quant Time: Feb 22 15:03:40 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 22 11:00:59 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	365	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	1540	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.49	164	915	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.23	188	1741m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.39	240	1214	0.40	ng/ul	0.00
20) Perylene-d12	23.61	264	1223	0.40	ng/ul	0.00

02/24/21 JU

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.23	152	957	0.44	ng/ul	0.00
14) Fluoranthene-d10	19.25	212	1704	0.38	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed