


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022221\
 Data File : BM028857.D
 Acq On : 22 Feb 2021 09:03
 Operator : CG/JU
 Sample : DFTPP35
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP35

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM020521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 22 11:00:59 2021

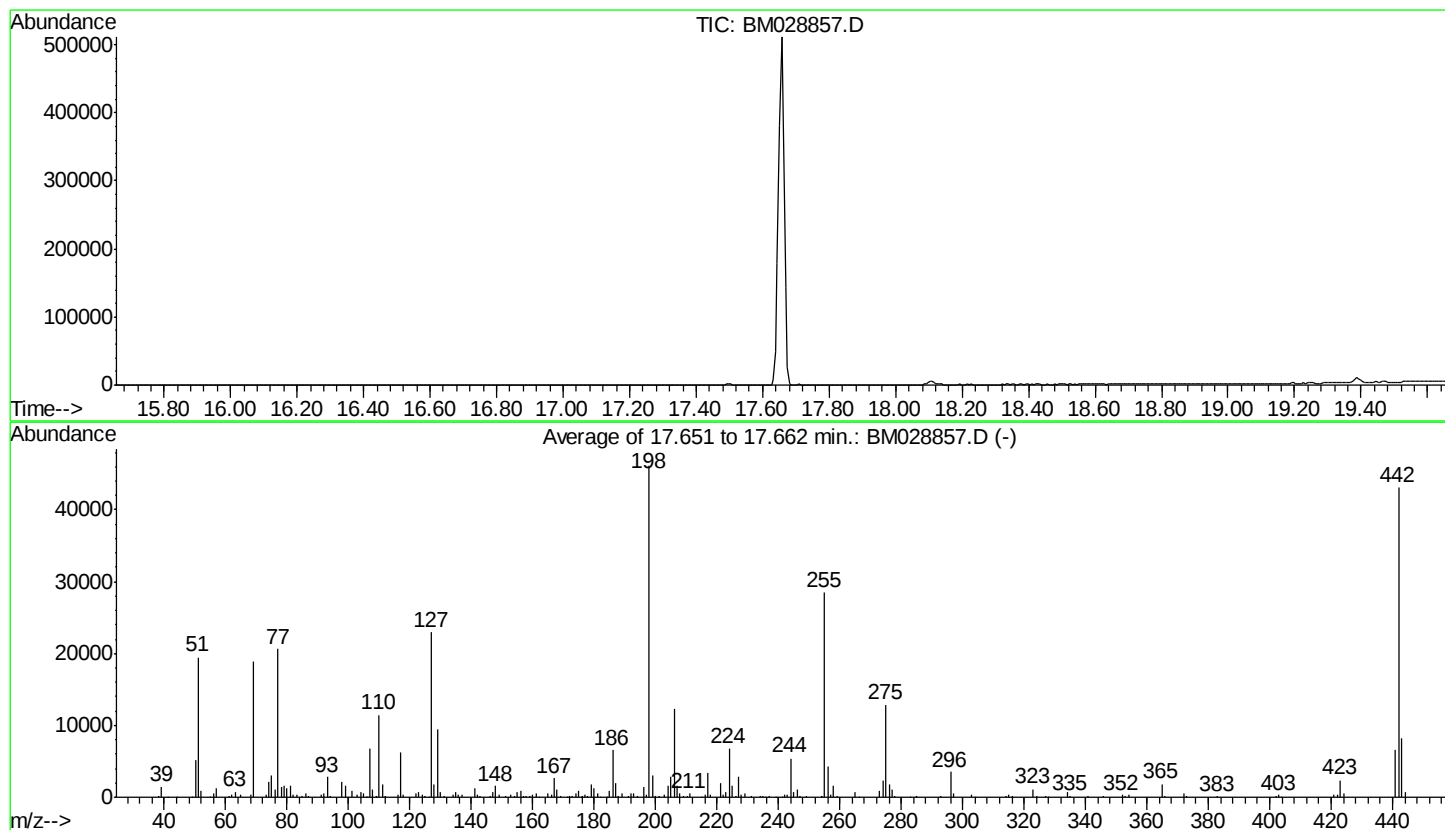

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.1	19434	PASS
68	69	0.00	2	1.8	337	PASS
69	198	0.00	100	41.0	18899	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.7	22954	PASS
197	198	0.00	2	0.6	284	PASS
198	198	100	100	100.0	46144	PASS
199	198	5	9	6.6	3066	PASS
275	198	10	60	27.9	12864	PASS
365	198	1	100	4.0	1858	PASS
441	198	0.01	100	14.3	6603	PASS
442	198	50	100	93.4	43098	PASS
443	442	15	24	19.2	8273	PASS

m/z	Abundance
38.00	255.0
39.10	1512.0
44.00	242.0
49.10	175.0
50.10	5496.0
51.10	20056.0
52.00	1087.0
56.00	591.0
57.00	1383.0
61.00	248.0
62.00	302.0
63.00	747.0
65.00	329.0
68.10	406.0
69.00	19424.0
73.00	334.0
74.00	2096.0
75.00	3111.0
76.10	1001.0
77.10	20840.0
78.10	1478.0
79.00	1506.0
80.00	1165.0
81.00	1747.0
82.00	312.0
83.00	264.0
85.00	247.0
86.00	480.0
87.00	207.0
91.00	374.0
92.00	479.0
93.00	2650.0
93.90	164.0
98.00	2141.0
99.00	1480.0
101.00	845.0
103.00	301.0
104.00	628.0
104.90	551.0
107.00	6585.0
108.00	965.0
109.20	262.0
110.00	11051.0
111.00	1845.0
111.90	226.0
116.10	446.0
117.00	5899.0
118.00	453.0
122.00	456.0
123.00	602.0
123.90	282.0
125.00	295.0
127.00	22032.0
128.00	1752.0
129.00	8969.0
130.00	811.0
131.00	205.0
134.00	241.0
135.00	719.0
135.90	276.0
136.90	396.0
141.00	1251.0
142.00	341.0
142.90	252.0
145.90	160.0
147.00	656.0
148.00	1611.0
149.00	352.0
151.00	182.0
153.00	332.0
154.00	207.0
155.00	695.0
156.00	825.0
157.10	165.0
157.90	228.0
159.00	212.0
159.90	387.0
161.00	553.0
164.90	472.0
166.10	294.0
167.00	2392.0
168.00	1102.0
169.00	266.0
172.00	225.0
173.10	249.0
173.90	541.0
175.00	842.0
175.90	250.0
177.00	387.0
177.90	175.0
179.00	1660.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35

180.00	1131.0
180.90	502.0
185.00	790.0
186.00	5867.0
187.00	1876.0
188.00	192.0
188.90	380.0
191.00	245.0
191.90	552.0
193.00	618.0
193.90	158.0
196.00	1484.0
198.00	42080.0
199.00	2905.0
199.90	234.0
201.20	154.0
203.00	277.0
204.00	1589.0
205.00	2680.0
206.00	11384.0
207.00	1761.0
207.90	448.0
208.90	192.0
211.00	415.0
216.00	284.0
217.00	2924.0
218.00	423.0
221.00	1642.0
221.90	376.0
223.00	692.0
224.00	5911.0
225.00	1461.0
226.00	161.0
227.00	2723.0
228.00	374.0
229.00	556.0
231.00	237.0
234.00	195.0
237.00	253.0
242.00	342.0
243.00	319.0
244.00	4629.0
245.00	635.0
246.00	872.0
247.00	161.0
249.00	172.0
254.00	230.0
255.00	23728.0
256.00	3522.0
256.90	267.0
258.00	1342.0
258.90	269.0
265.00	575.0
273.00	647.0
274.00	1977.0
275.00	10661.0
276.00	1555.0
277.00	909.0
277.90	180.0
284.90	180.0
293.00	201.0
296.00	2883.0
297.00	439.0
303.00	326.0
315.00	381.0
316.00	191.0
323.00	804.0
323.90	208.0
326.90	200.0
334.00	545.0
335.00	160.0
340.90	154.0
345.90	228.0
352.00	261.0
354.00	293.0
364.90	1290.0
366.00	210.0
372.00	448.0
403.00	345.0
420.90	248.0
422.00	202.0
423.00	1722.0
424.00	451.0
441.00	4386.0
442.00	30016.0
443.00	5904.0
444.00	604.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35

m/z	Abundance
38.00	332.0
39.00	1773.0
41.00	150.0
44.00	205.0
50.10	6218.0
51.10	23640.0
52.10	1181.0
55.00	179.0
56.00	758.0
57.00	1540.0
60.90	243.0
62.00	319.0
63.00	830.0
65.00	424.0
68.00	358.0
69.00	22728.0
73.00	433.0
74.00	2532.0
75.00	3559.0
76.00	1247.0
77.10	25064.0
78.00	1691.0
79.00	1842.0
80.00	1384.0
81.00	1886.0
82.00	441.0
83.00	400.0
85.00	291.0
86.00	559.0
86.90	274.0
91.00	486.0
92.00	513.0
93.00	3437.0
93.90	229.0
98.00	2623.0
99.00	1935.0
101.00	1031.0
102.90	351.0
104.00	778.0
105.00	699.0
106.20	230.0
107.00	8349.0
108.00	1227.0
108.90	262.0
110.00	13795.0
111.00	2177.0
112.10	286.0
116.00	496.0
117.00	7601.0
118.00	541.0
122.00	603.0
123.00	822.0
124.00	386.0
124.90	314.0
127.00	27768.0
128.00	2192.0
129.00	11578.0
130.00	862.0
131.10	202.0
134.00	359.0
135.00	1041.0
135.90	379.0
137.00	499.0
141.00	1662.0
141.90	474.0
142.90	298.0
146.00	263.0
146.90	867.0
148.00	1805.0
149.00	308.0
151.10	202.0
153.00	448.0
154.00	292.0
155.10	771.0
156.00	1126.0
157.00	227.0
158.00	273.0
158.90	207.0
160.00	509.0
161.00	671.0
161.90	184.0
165.00	677.0
166.00	424.0
167.00	3341.0
168.00	1364.0
169.00	251.0
171.00	158.0
172.00	290.0
172.90	302.0
174.00	588.0
175.00	1095.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35

176.10	310.0
177.00	555.0
178.00	187.0
179.00	2162.0
180.00	1517.0
181.00	627.0
182.10	160.0
183.90	209.0
185.00	980.0
186.00	8013.0
187.00	2241.0
187.90	227.0
189.00	646.0
190.90	368.0
192.00	697.0
193.00	756.0
194.00	181.0
196.00	1706.0
197.10	521.0
198.00	55448.0
199.00	3679.0
200.00	297.0
201.30	242.0
203.00	453.0
204.00	1860.0
205.00	3370.0
206.00	14392.0
207.00	2223.0
208.00	587.0
209.00	178.0
210.20	319.0
211.00	663.0
216.00	420.0
217.00	4107.0
218.00	465.0
221.00	2386.0
221.80	491.0
223.00	828.0
224.00	7945.0
225.10	1971.0
226.10	177.0
227.00	3318.0
228.00	503.0
229.00	693.0
231.10	288.0
233.90	196.0
235.00	281.0
235.90	198.0
236.90	298.0
239.00	178.0
241.00	177.0
242.00	378.0
243.00	517.0
244.10	6300.0
245.00	884.0
246.00	1307.0
247.00	289.0
249.00	252.0
254.20	326.0
255.00	34184.0
256.00	5255.0
257.00	372.0
258.00	2065.0
258.90	330.0
265.00	815.0
266.00	153.0
273.00	1045.0
274.00	2828.0
275.00	15338.0
276.00	2223.0
277.00	1265.0
277.90	236.0
283.00	164.0
285.10	262.0
292.90	262.0
296.00	4228.0
297.00	594.0
302.90	481.0
314.00	214.0
315.00	485.0
316.00	228.0
323.00	1238.0
324.00	260.0
326.90	253.0
328.00	164.0
334.00	879.0
335.00	232.0
341.00	196.0
346.00	294.0
352.00	370.0
353.00	260.0
353.90	451.0
365.00	2127.0
365.90	268.0
372.00	632.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35

373.00	175.0
383.00	208.0
401.90	224.0
402.90	416.0
403.90	172.0
421.00	352.0
422.00	450.0
423.00	2575.0
424.00	615.0
441.00	7882.0
442.00	50200.0
443.00	9768.0
444.00	909.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35

m/z	Abundance
38.00	200.0
39.00	1110.0
44.00	265.0
50.00	3851.0
51.10	14608.0
52.00	682.0
56.00	426.0
57.00	1021.0
62.00	222.0
63.00	605.0
65.00	282.0
68.10	247.0
69.00	14546.0
73.00	276.0
74.00	1633.0
75.00	2446.0
76.10	757.0
77.10	16043.0
78.00	1176.0
79.10	1301.0
80.00	969.0
81.00	1190.0
82.00	309.0
83.00	290.0
84.90	192.0
85.90	373.0
86.90	195.0
91.00	353.0
92.00	423.0
93.00	2241.0
98.00	1724.0
99.00	1195.0
101.00	645.0
103.00	261.0
104.00	508.0
105.00	478.0
105.90	161.0
107.00	5415.0
108.00	947.0
109.00	242.0
110.00	9377.0
111.00	1411.0
112.00	173.0
116.00	318.0
117.00	5060.0
118.00	306.0
122.00	369.0
123.00	598.0
123.90	224.0
124.90	211.0
126.20	218.0
127.00	19064.0
128.00	1569.0
129.00	7745.0
130.00	622.0
131.00	174.0
133.90	240.0
135.00	608.0
135.90	293.0
137.00	276.0
141.00	1074.0
142.00	403.0
143.00	237.0
145.90	210.0
146.90	587.0
148.00	1297.0
148.90	322.0
151.10	183.0
153.00	253.0
153.90	228.0
155.00	665.0
156.00	761.0
156.90	213.0
157.90	215.0
158.90	171.0
159.90	387.0
160.90	509.0
165.00	423.0
165.90	359.0
167.00	2189.0
168.00	972.0
169.00	253.0
173.00	249.0
173.90	464.0
175.00	854.0
176.00	259.0
177.00	375.0
179.00	1627.0
180.00	1209.0
181.00	440.0
185.00	862.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35

186.00	5785.0
187.00	1683.0
188.00	224.0
188.90	400.0
190.90	184.0
192.00	593.0
193.00	471.0
196.00	1184.0
197.10	332.0
198.00	40904.0
199.00	2614.0
199.90	272.0
201.30	240.0
203.00	317.0
204.00	1566.0
205.00	2734.0
206.00	11225.0
207.00	1557.0
208.00	436.0
211.00	459.0
214.90	158.0
216.00	280.0
217.00	3059.0
218.00	383.0
221.00	1872.0
221.80	481.0
223.00	566.0
224.00	6418.0
225.00	1609.0
226.00	187.0
227.00	2498.0
227.90	429.0
229.00	555.0
231.00	192.0
233.90	198.0
235.00	223.0
237.00	188.0
242.00	311.0
243.00	392.0
244.00	5123.0
245.00	695.0
246.00	998.0
246.90	169.0
249.00	190.0
255.00	27368.0
256.00	3918.0
256.90	348.0
258.00	1556.0
259.00	216.0
265.00	615.0
273.00	924.0
274.00	2070.0
275.00	12594.0
276.00	1708.0
277.00	1102.0
278.00	189.0
284.90	185.0
293.00	267.0
296.00	3504.0
297.00	522.0
303.00	413.0
303.90	154.0
313.90	178.0
314.90	410.0
323.00	1176.0
324.00	237.0
327.00	213.0
334.00	798.0
335.00	187.0
341.00	199.0
345.80	216.0
351.90	340.0
353.00	218.0
354.00	463.0
365.00	2157.0
365.90	252.0
372.00	630.0
373.00	161.0
383.00	196.0
402.00	317.0
403.00	311.0
421.00	360.0
422.00	402.0
423.00	2702.0
424.00	599.0
441.00	7542.0
442.00	49080.0
443.00	9149.0
444.00	819.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35

Scan 2487 (17.615 min): BM028857.D
DFTPP35

m/z	Abundance
44.00	220.0
206.90	193.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35