

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022316\
 Data File : BM004364.D
 Acq On : 23 Feb 2016 23:46
 Operator : SJ/UM
 Sample : H1542-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-S28-0003

Quant Time: Feb 24 02:57:51 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 24 02:51:42 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	26722	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	115696	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.28	164	62648	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	130248	20.00	ng/ul	0.00
78) Chrysene-d12	21.24	240	132938	20.00	ng/ul	0.00
86) Perylene-d12	23.46	264	132453	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.09	96	3459	6.82	ng/uL	0.00
5) Phenol-d5	6.81	99	68647	30.64	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	38977	34.20	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	64991	33.63	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	56942	28.44	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	30819	35.01	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	34982	34.86	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	56868	31.36	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	70907	31.37	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	181326	33.75	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	226766	36.05	ng/ul	0.00
52) 4-Nitrophenol-d4	14.53	143	19566	22.66	ng/ul	0.00
58) Fluorene-d10	15.28	176	155407	34.01	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.43	200	20372	25.46	ng/ul	0.00
71) Anthracene-d10	17.13	188	231532	36.28	ng/ul	0.00
79) Pyrene-d10	19.44	212	252822	39.32	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.33	264	258554	37.20	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.75	163	47617	8.50	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022316\
Data File : BM004364.D
Acq On : 23 Feb 2016 23:46
Operator : SJ/UM
Sample : H1542-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0311-S28-0003

Quant Time: Feb 24 02:57:51 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 24 02:51:42 2016
Response via : Initial Calibration

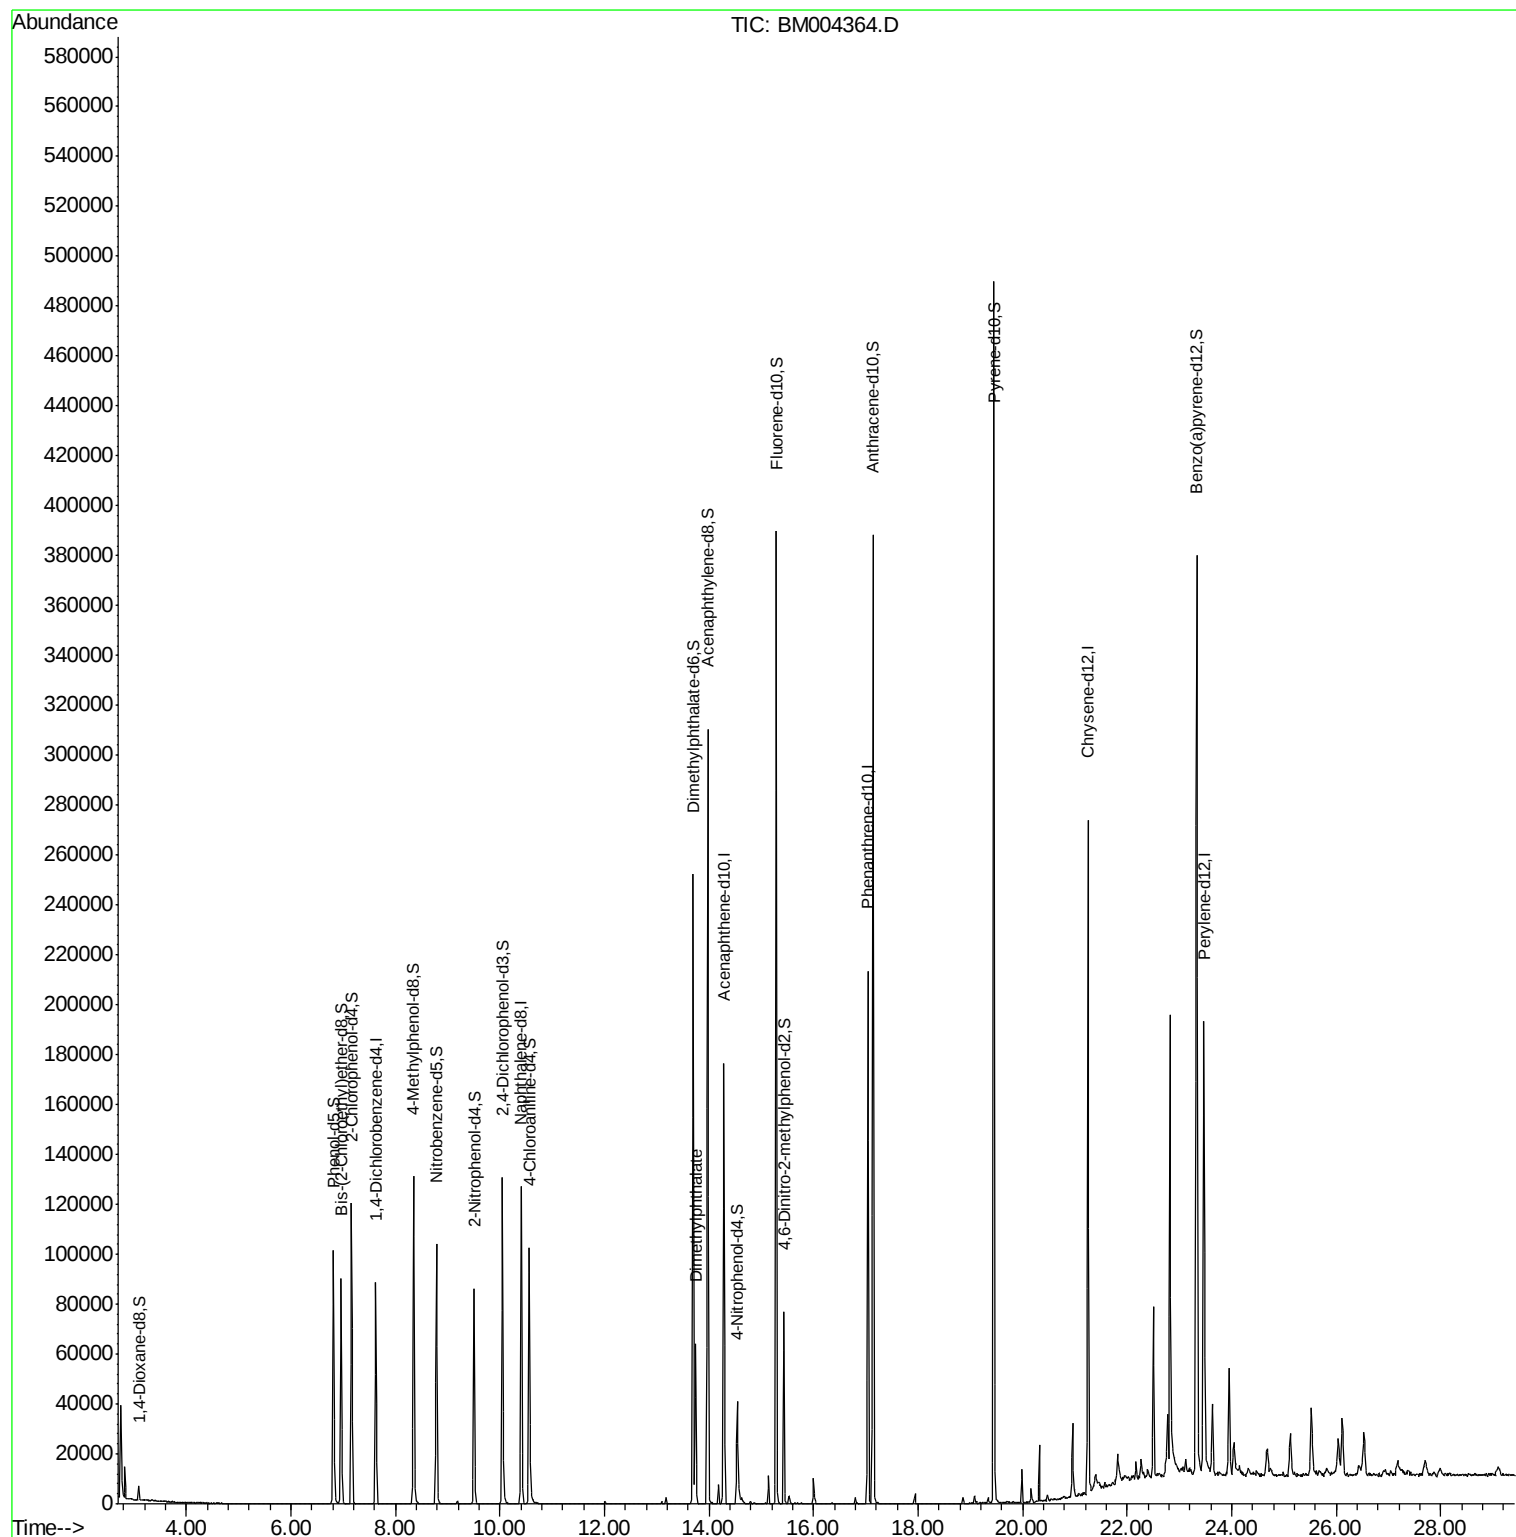

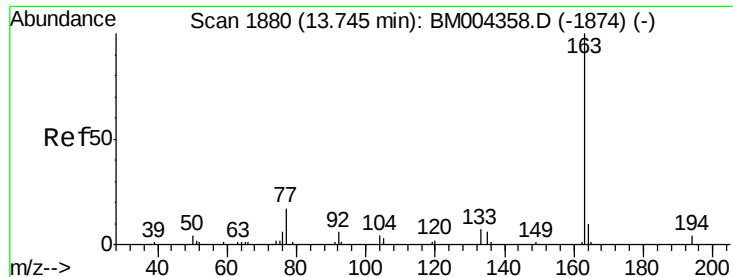

#45

Dimethylphthalate

Concen: 8.50 ng/ul

RT: 13.75 min Scan# 1880

Delta R.T. 0.00 min

Lab File: BM004364.D


Acq: 23 Feb 2016 23:46

Instrument :

BNA_M

ClientSampleId :

0311-S28-0003

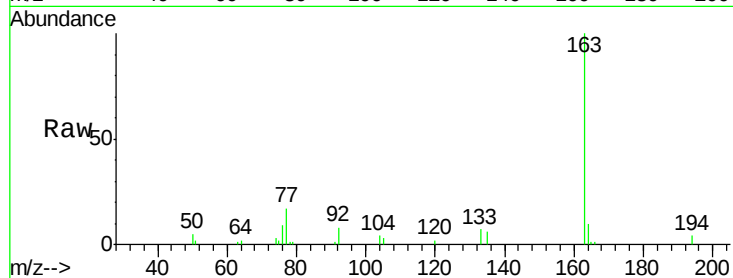

Tgt Ion:	163	Resp:	47617
Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.2	4.8
164	10.2	7.8	11.8

