


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022316\
Data File : BM004340.D
Acq On : 23 Feb 2016 09:16
Operator : SJ/UM
Sample : DFTPP54
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Title : SVOA CALIBRATION
Last Update : Wed Feb 24 12:04:45 2016

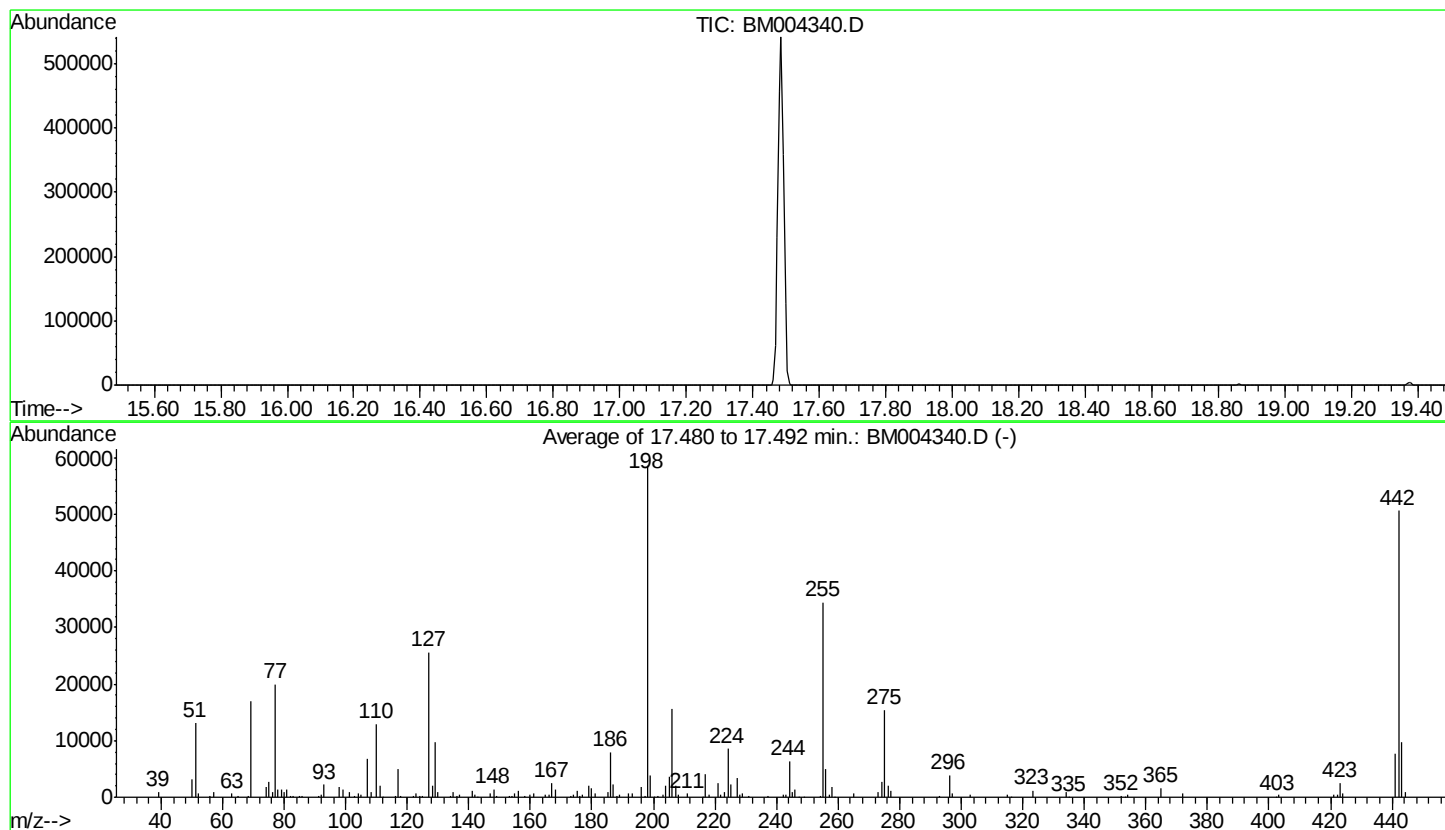

AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.5	13207	PASS
68	69	0.00	2	1.4	229	PASS
69	198	0.00	100	28.9	16947	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.6	25570	PASS
197	198	0.00	2	0.5	301	PASS
198	198	100	100	100.0	58605	PASS
199	198	5	9	6.7	3923	PASS
275	198	10	60	26.4	15484	PASS
365	198	1	100	2.8	1640	PASS
441	443	0.01	100	79.6	7711	PASS
442	198	50	100	86.5	50666	PASS
443	442	15	24	19.1	9691	PASS