

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022316\
 Data File : BM004346.D
 Acq On : 23 Feb 2016 12:55
 Operator : SJ/UM
 Sample : H1515-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-S26-0312

Manual Integrations
 APPROVED

UMANGI
 2/24/2016 4:30:35 PM

Quant Time: Feb 24 01:29:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 24 01:02:10 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	28595	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	138792	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	87106	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	200554	20.00	ng/ul	0.00
78) Chrysene-d12	21.25	240	193472	20.00	ng/ul	0.00
86) Perylene-d12	23.47	264	141360	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.09	96	2762	5.09	ng/uL	0.00
5) Phenol-d5	6.82	99	57136m	23.83	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	34009	27.89	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	53117	25.68	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	44033	20.55	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	26896	25.47	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	30053	24.97	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	51654m	23.74	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	73850	27.23	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	200848	26.89	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	235098	26.88	ng/ul	0.00
52) 4-Nitrophenol-d4	14.53	143	19637m	16.35	ng/ul	0.00
58) Fluorene-d10	15.29	176	171757	27.04	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.43	200	20905	16.97	ng/ul	0.00
71) Anthracene-d10	17.14	188	271732	27.65	ng/ul	0.00
79) Pyrene-d10	19.44	212	301488	32.22	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.33	264	210594	28.39	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.74	163	48186	6.19	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022316\
Data File : BM004346.D
Acq On : 23 Feb 2016 12:55
Operator : SJ/UM
Sample : H1515-04
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
0311-S26-0312

Manual Integrations
APPROVED

UMANGI
2/24/2016 4:30:35 PM

Quant Time: Feb 24 01:29:15 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 24 01:02:10 2016
Response via : Initial Calibration

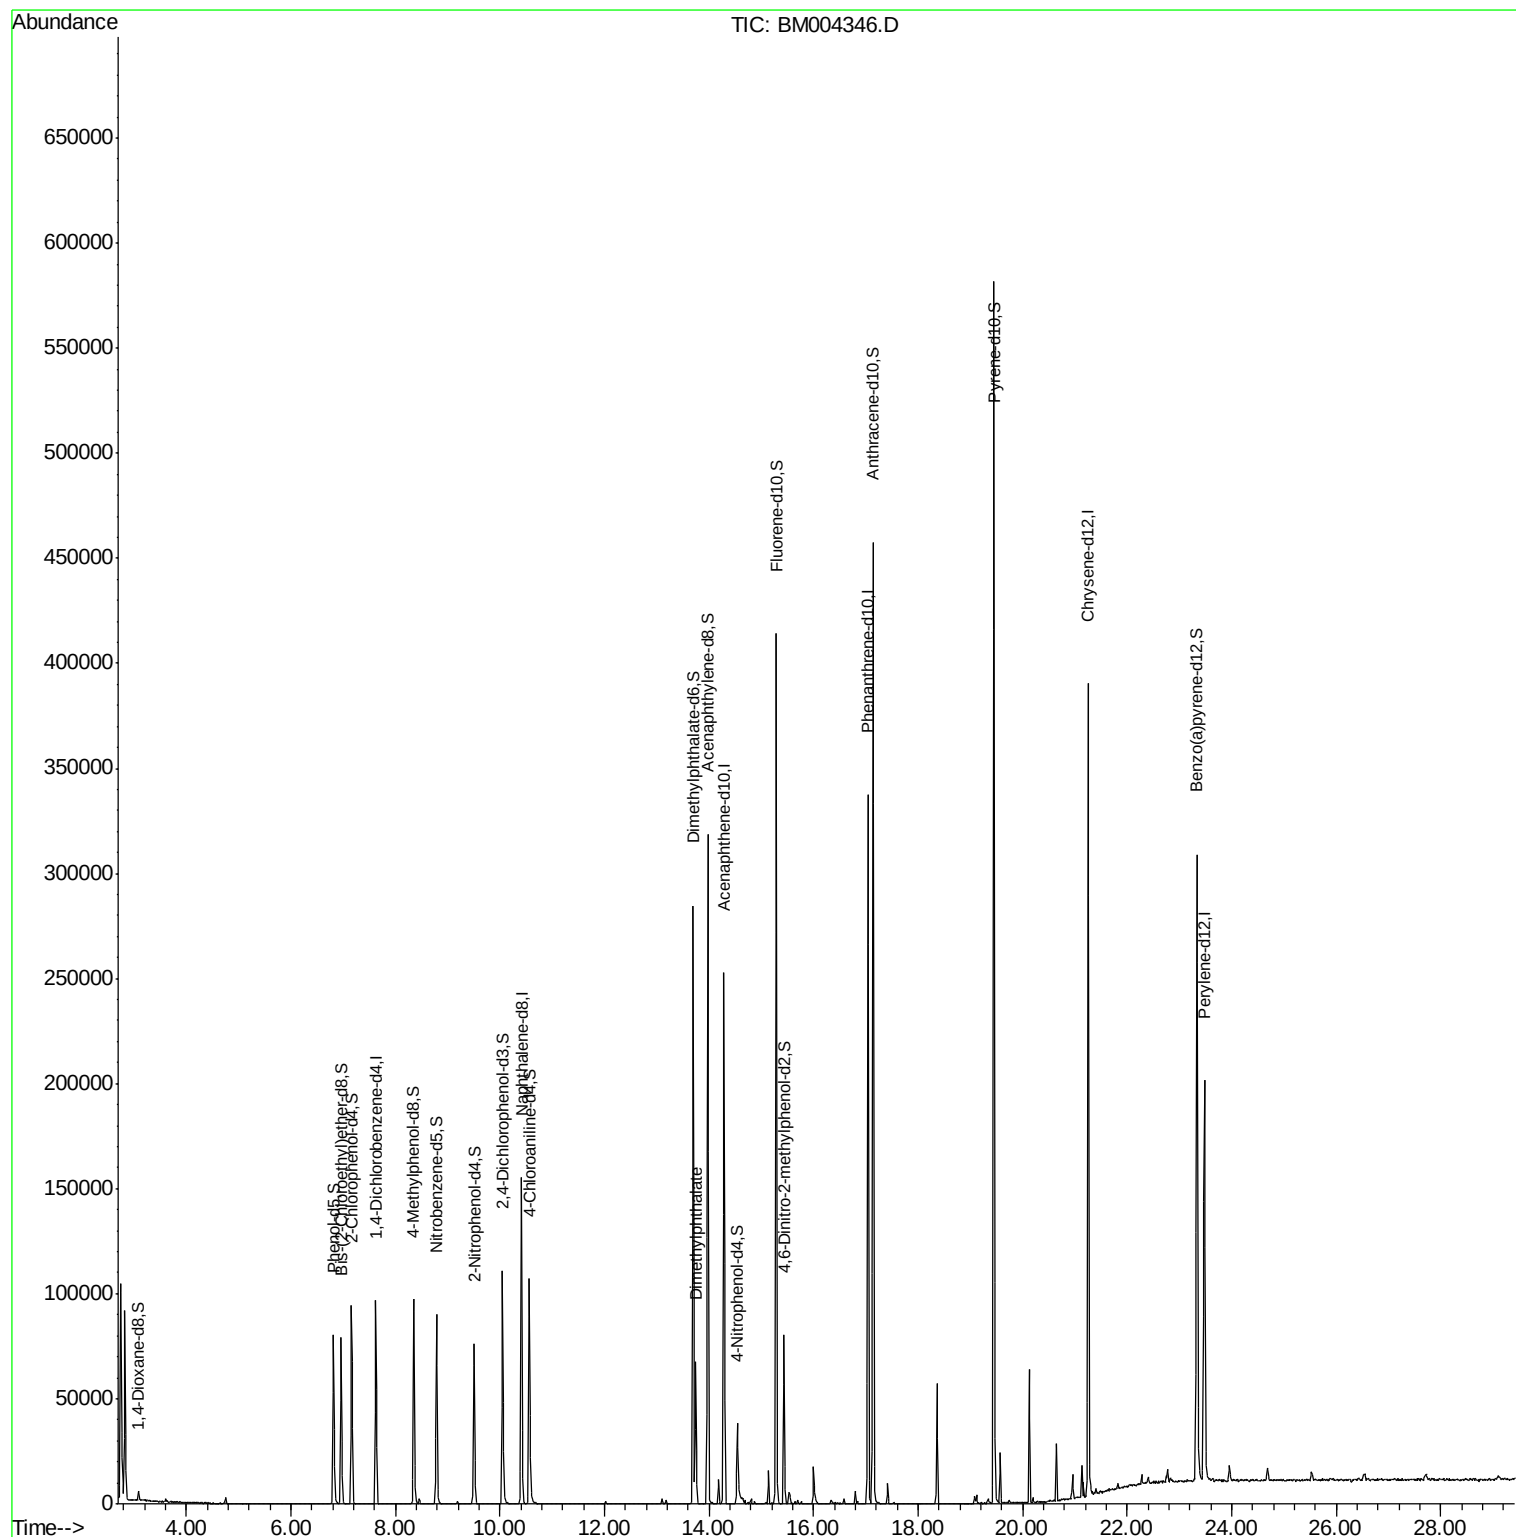

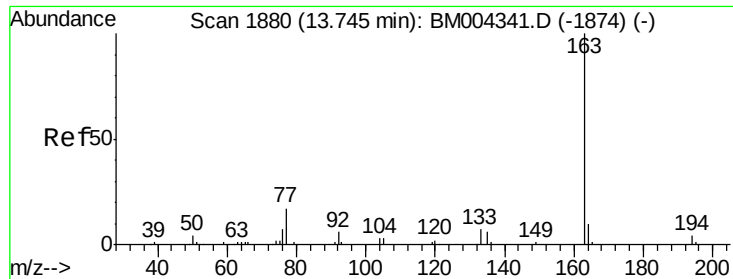

#45

Dimethylphthalate

Concen: 6.19 ng/ul

RT: 13.74 min Scan# 1880

Delta R.T. -0.00 min

Lab File: BM004346.D


Acq: 23 Feb 2016 12:55

Instrument :

BNA_M

ClientSampleId :

0311-S26-0312

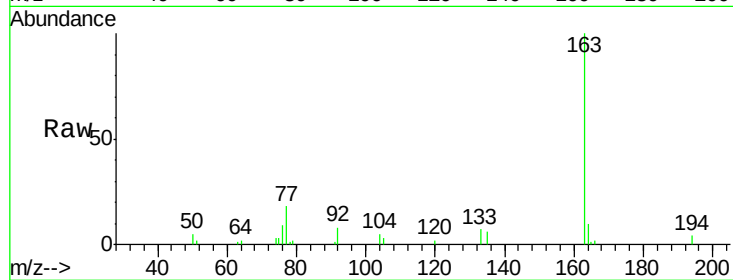

Tgt Ion:	163	Resp:	48186
Ion Ratio	Lower	Upper	
163	100		
194	4.1	3.2	4.8
164	9.8	7.8	11.8

Manual Integrations
APPROVED

UMANGI
2/24/2016 4:30:35 PM

