

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022316\
 Data File : BM004348.D
 Acq On : 23 Feb 2016 14:07
 Operator : SJ/UM
 Sample : H1515-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-S17-0003

Manual Integrations
 APPROVED

UMANGI
 2/24/2016 4:30:41 PM

Quant Time: Feb 24 01:34:24 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 24 01:02:10 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	26158	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	121786	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	76556	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	181990	20.00	ng/ul	0.00
78) Chrysene-d12	21.25	240	194989	20.00	ng/ul	0.00
86) Perylene-d12	23.47	264	149313	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.09	96	2723	5.49	ng/uL	0.00
5) Phenol-d5	6.82	99	54156m	24.69	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	30725	27.54	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	49702	26.27	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	46657	23.80	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	24263	26.19	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	27818	26.34	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	47436m	24.85	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	71662m	30.12	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	182479	27.79	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	214393	27.89	ng/ul	0.00
52) 4-Nitrophenol-d4	14.53	143	18814m	17.83	ng/ul	0.00
58) Fluorene-d10	15.28	176	158544	28.40	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.43	200	20252	18.12	ng/ul	0.00
71) Anthracene-d10	17.14	188	250280	28.07	ng/ul	0.00
79) Pyrene-d10	19.44	212	287302	30.46	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.33	264	222285	28.37	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.74	163	44978	6.57	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022316\
Data File : BM004348.D
Acq On : 23 Feb 2016 14:07
Operator : SJ/UM
Sample : H1515-11
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
0311-S17-0003

Manual Integrations
APPROVED

UMANGI
2/24/2016 4:30:41 PM

Quant Time: Feb 24 01:34:24 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 24 01:02:10 2016
Response via : Initial Calibration

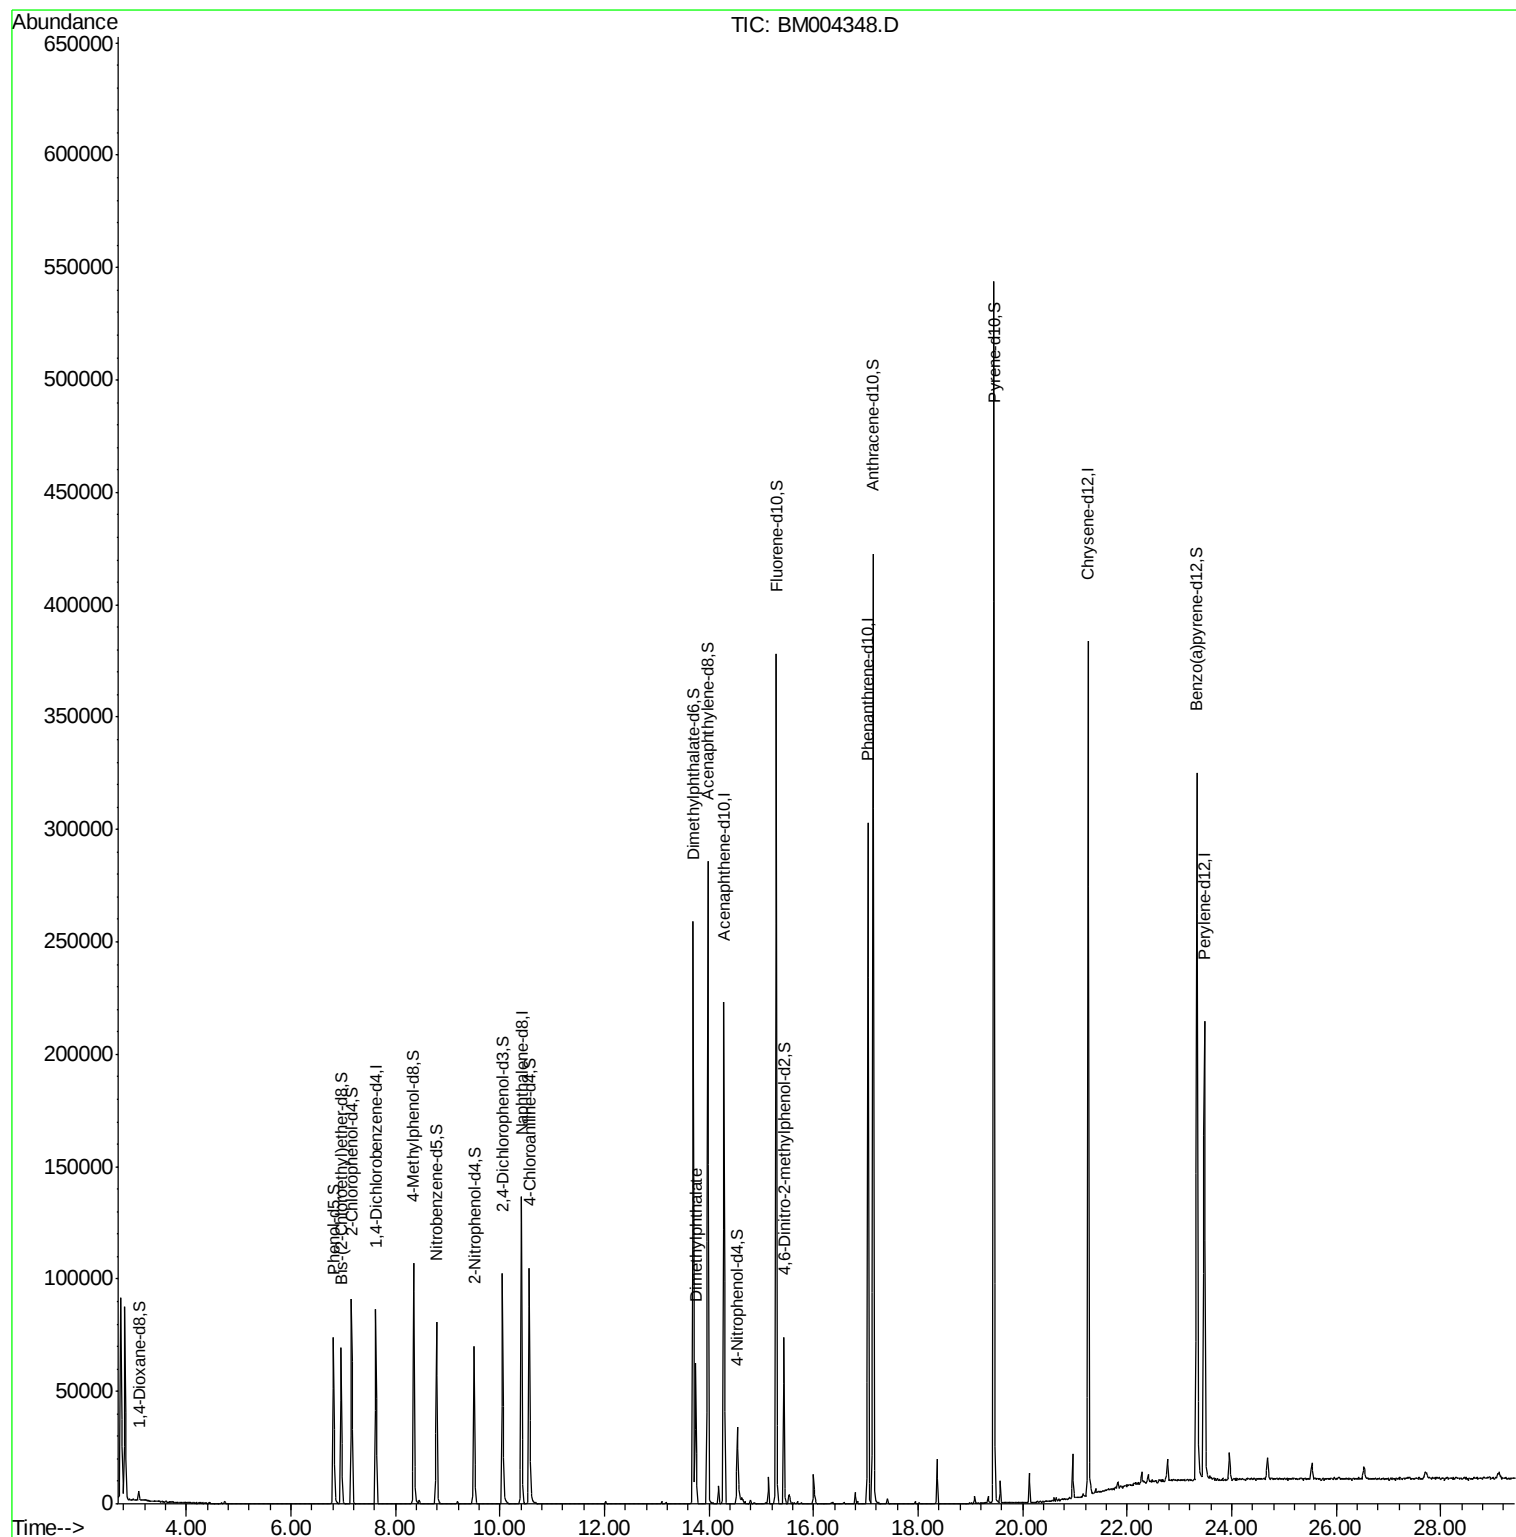

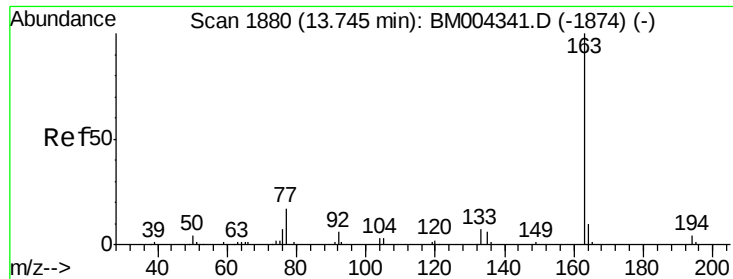


#45
 Dimethylphthalate
 Concen: 6.57 ng/ul
 RT: 13.74 min Scan# 1880
 Delta R.T. -0.00 min
 Lab File: BM004348.D
 Acq: 23 Feb 2016 14:07

Instrument :
 BNA_M
 ClientSampleId :
 0311-S17-0003

Tgt Ion:	163	Resp:	44978
Ion Ratio	Lower	Upper	
163	100		
194	4.3	3.2	4.8
164	10.2	7.8	11.8

Manual Integrations
 APPROVED

UMANGI
 2/24/2016 4:30:41 PM

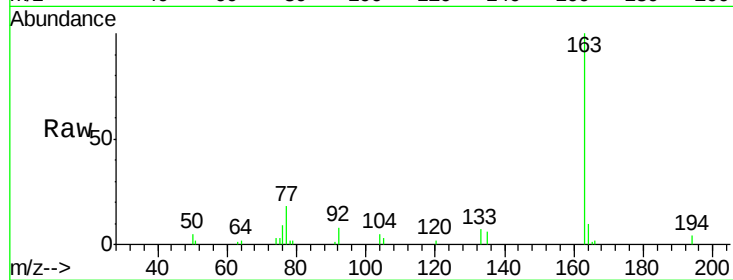

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

