


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022316\
Data File : BM004340.D
Acq On : 23 Feb 2016 09:16
Operator : SJ/UM
Sample : DFTPP54
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP54

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Title : SVOA CALIBRATION
Last Update : Wed Feb 24 12:04:45 2016

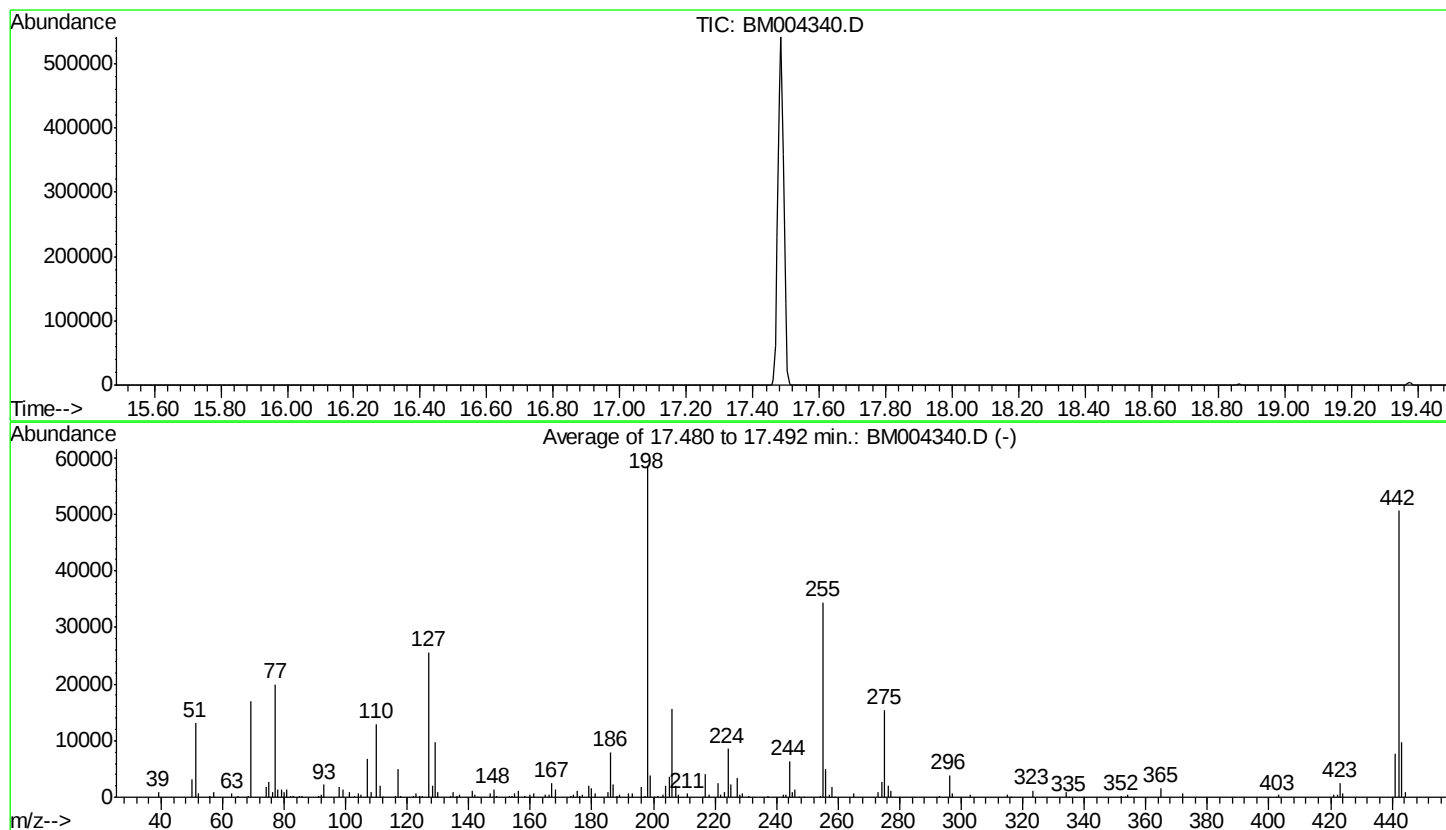

AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.5	13207	PASS
68	69	0.00	2	1.4	229	PASS
69	198	0.00	100	28.9	16947	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.6	25570	PASS
197	198	0.00	2	0.5	301	PASS
198	198	100	100	100.0	58605	PASS
199	198	5	9	6.7	3923	PASS
275	198	10	60	26.4	15484	PASS
365	198	1	100	2.8	1640	PASS
441	443	0.01	100	79.6	7711	PASS
442	198	50	100	86.5	50666	PASS
443	442	15	24	19.1	9691	PASS

m/z	Abundance
39.00	1160.0
50.10	3747.0
51.10	15135.0
52.10	843.0
56.00	486.0
57.00	1048.0
63.10	684.0
65.00	386.0
68.10	331.0
69.00	19304.0
74.00	1951.0
75.00	3109.0
76.10	1092.0
77.10	22384.0
78.10	1556.0
79.00	1561.0
80.00	1108.0
81.00	1658.0
82.00	407.0
83.00	354.0
85.00	424.0
86.00	456.0
91.00	319.0
92.00	479.0
93.00	2426.0
98.00	1992.0
99.00	1589.0
101.00	1042.0
103.00	339.0
104.00	668.0
105.00	576.0
107.10	7653.0
108.00	1144.0
110.00	14068.0
111.00	2198.0
116.00	485.0
117.00	5553.0
118.00	407.0
122.00	448.0
123.00	793.0
124.00	360.0
125.10	331.0
127.10	27704.0
128.00	2248.0
129.00	10193.0
130.00	893.0
135.00	893.0
136.00	400.0
137.10	435.0
141.00	1359.0
142.00	453.0
147.00	762.0
148.00	1569.0
149.00	329.0
153.00	501.0
153.90	328.0
155.00	817.0
156.00	1277.0
158.00	311.0
160.00	377.0
161.00	657.0
165.00	516.0
166.00	412.0
167.10	2834.0
168.10	1516.0
173.00	348.0
174.00	545.0
175.00	1046.0
176.00	355.0
177.00	528.0
179.00	2103.0
180.00	1690.0
181.00	711.0
185.10	1032.0
186.10	8195.0
187.10	2407.0
188.00	336.0
189.00	516.0
192.00	638.0
193.00	736.0
196.10	1702.0
197.10	461.0
198.00	60568.0
199.00	4100.0
203.00	380.0
204.10	2113.0
205.10	3622.0
206.10	16190.0
207.10	2254.0
208.00	458.0
211.10	585.0

Instrument :
BNA_M
ClientSampleId :
DFTPP54

217.00	3993.0
218.00	517.0
221.10	2361.0
221.80	645.0
223.10	915.0
224.10	8058.0
225.10	2100.0
227.10	3290.0
228.00	517.0
229.10	686.0
237.10	415.0
242.10	459.0
243.10	367.0
244.10	6395.0
245.10	880.0
246.00	1248.0
254.20	364.0
255.10	33624.0
256.10	5042.0
257.00	423.0
258.00	1818.0
265.00	710.0
273.10	914.0
274.10	2543.0
275.10	14578.0
276.10	2077.0
277.00	1113.0
293.00	329.0
296.10	3648.0
297.00	586.0
303.10	412.0
315.10	347.0
323.10	1151.0
334.10	809.0
354.10	389.0
365.10	1398.0
372.10	556.0
403.00	356.0
421.10	319.0
422.20	328.0
423.10	2074.0
424.10	722.0
441.20	6030.0
442.20	39992.0
443.10	7912.0
444.10	718.0

Instrument :
BNA_M
ClientSampleId :
DFTPP54

m/z	Abundance
39.10	1088.0
50.10	3884.0
51.10	15635.0
52.00	779.0
56.00	430.0
57.00	1149.0
63.00	769.0
65.10	446.0
68.20	357.0
69.00	19912.0
74.00	1992.0
75.00	3197.0
76.10	1065.0
77.10	23456.0
78.10	1419.0
79.00	1562.0
80.00	1251.0
81.00	1682.0
82.00	415.0
83.00	405.0
85.00	454.0
86.00	470.0
91.00	413.0
92.10	472.0
93.00	2601.0
98.00	2006.0
99.00	1708.0
101.00	1054.0
103.10	344.0
104.00	701.0
105.00	613.0
107.00	8069.0
108.00	1126.0
110.00	15472.0
111.00	2324.0
112.00	316.0
116.00	366.0
117.00	6018.0
118.00	442.0
122.10	472.0
123.00	886.0
123.90	413.0
125.00	332.0
127.10	30416.0
128.10	2276.0
129.00	11617.0
130.00	1099.0
133.90	396.0
135.00	941.0
136.00	387.0
137.10	548.0
141.00	1492.0
142.10	501.0
142.90	313.0
147.00	731.0
148.00	1632.0
149.00	345.0
153.00	494.0
154.00	422.0
155.00	846.0
156.00	1386.0
158.00	313.0
160.00	498.0
161.00	699.0
165.00	573.0
166.10	433.0
167.00	3065.0
168.00	1403.0
173.00	366.0
174.00	698.0
175.10	1261.0
176.00	357.0
177.00	649.0
179.00	2391.0
180.00	1785.0
181.00	795.0
185.00	1164.0
186.10	9473.0
187.00	2806.0
188.00	353.0
189.00	575.0
192.00	709.0
193.00	889.0
196.00	2139.0
197.10	444.0
198.00	69192.0
199.00	4700.0
200.00	319.0
201.50	368.0
203.10	529.0
204.10	2553.0

Instrument :
BNA_M
ClientSampleId :
DFTPP54

205.10	4268.0
206.10	18416.0
207.10	2549.0
208.00	625.0
211.10	701.0
216.10	353.0
217.00	4798.0
218.00	627.0
221.10	2839.0
223.10	1089.0
224.10	10388.0
225.10	2575.0
227.10	3877.0
228.00	550.0
229.10	787.0
231.00	383.0
237.10	370.0
242.10	493.0
243.10	506.0
244.10	7570.0
245.10	1117.0
246.00	1428.0
247.00	306.0
249.00	356.0
254.20	420.0
255.10	40952.0
256.10	6054.0
257.00	442.0
258.10	2164.0
259.00	360.0
265.00	874.0
273.10	1263.0
274.10	3170.0
275.10	18504.0
276.10	2558.0
277.00	1436.0
293.00	342.0
296.10	4559.0
297.00	657.0
303.00	448.0
315.00	460.0
316.10	330.0
323.10	1506.0
334.00	1022.0
335.00	300.0
352.10	444.0
353.10	331.0
354.10	491.0
365.10	1952.0
372.10	863.0
402.20	334.0
403.10	391.0
421.00	456.0
422.10	403.0
423.20	2984.0
424.20	804.0
441.20	9328.0
442.20	60240.0
443.10	11428.0
444.20	1127.0

Instrument :
BNA_M
ClientSampleId :
DFTPP54

m/z	Abundance
39.00	564.0
50.10	2142.0
51.10	8853.0
52.10	403.0
57.00	625.0
63.00	496.0
69.00	11627.0
74.00	1286.0
75.00	1874.0
76.10	640.0
77.10	14028.0
78.00	984.0
79.00	934.0
80.00	700.0
81.00	1050.0
92.00	307.0
93.00	1561.0
98.00	1236.0
99.00	1040.0
101.00	644.0
104.00	353.0
105.00	361.0
107.10	4786.0
108.10	770.0
110.00	9420.0
111.00	1329.0
117.00	3665.0
123.00	495.0
127.10	18592.0
128.00	1431.0
129.00	7190.0
130.00	575.0
135.10	592.0
137.00	364.0
141.00	898.0
142.00	352.0
147.00	482.0
148.00	998.0
155.00	557.0
156.00	821.0
160.00	311.0
161.00	457.0
165.00	399.0
166.00	322.0
167.00	1719.0
168.00	935.0
174.10	421.0
175.10	848.0
177.00	388.0
179.00	1567.0
180.00	1217.0
181.10	458.0
185.10	722.0
186.10	6216.0
187.00	1810.0
189.00	373.0
192.00	477.0
193.00	517.0
196.10	1345.0
198.00	46056.0
199.00	2970.0
203.00	371.0
204.00	1608.0
205.10	2810.0
206.10	12177.0
207.10	1641.0
208.10	408.0
211.00	497.0
217.00	3150.0
218.00	356.0
221.10	2222.0
221.90	466.0
223.10	722.0
224.10	7045.0
225.10	1827.0
227.10	2798.0
228.10	434.0
229.00	601.0
242.00	302.0
243.10	311.0
244.10	5104.0
245.10	614.0
246.00	1123.0
255.10	28600.0
256.10	3890.0
257.00	313.0
258.00	1502.0
265.00	640.0
273.10	734.0
274.10	2213.0
275.10	13372.0

Instrument :
BNA_M
ClientSampleId :
DFTPP54

276.10	1689.0
277.10	1108.0
296.10	3415.0
297.10	527.0
303.10	378.0
315.10	326.0
323.10	1060.0
334.10	814.0
352.10	346.0
354.10	399.0
365.00	1570.0
372.10	723.0
403.10	345.0
421.10	375.0
422.10	330.0
423.10	2555.0
424.10	567.0
441.20	7775.0
442.20	51768.0
443.20	9735.0
444.10	866.0

Instrument :
BNA_M
ClientSampleId :
DFTPP54

Instrument :

BNA_M

ClientSampleId :

DFTPP54