

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM022318\
 Data File : BM014331.D
 Acq On : 23 Feb 2018 15:20
 Operator : SJ/JU
 Sample : PB106764BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Feb 23 15:52:17 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 22 03:35:18 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.53	152	68547	20.00	ng/ul	0.00
18) Naphthalene-d8	10.30	136	317744	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.18	164	211964	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.94	188	494253	20.00	ng/ul	0.00
75) Chrysene-d12	21.15	240	441869	20.00	ng/ul	0.00
83) Perylene-d12	23.32	264	424048	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.10	96	10066	6.29	ng/uL	0.00
5) Phenol-d5	6.72	99	154916	26.74	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.87	67	100608	28.69	ng/ul	0.00
9) 2-Chlorophenol-d4	7.06	132	119915	26.99	ng/ul	0.00
13) 4-Methylphenol-d8	8.25	113	127855	25.22	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	2137	0.91	ng/ul	0.05
22) 2-Nitrophenol-d4	9.40	143	70932	29.19	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.94	165	118589	23.56	ng/ul	0.00
29) 4-Chloroaniline-d4	10.46	131	162041	32.67	ng/ul	0.00
43) Dimethylphthalate-d6	13.60	166	595958	34.05	ng/ul	0.00
46) Acenaphthylene-d8	13.87	160	688315	31.89	ng/ul	0.00
51) 4-Nitrophenol-d4	14.44	143	39017	16.14	ng/ul	0.00
57) Fluorene-d10	15.19	176	517096	32.97	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.34	200	73480	24.78	ng/ul	0.00
70) Anthracene-d10	17.04	188	836080	35.06	ng/ul	0.00
76) Pyrene-d10	19.34	212	943261	41.39	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.19	264	706940	34.25	ng/ul	0.00

Target Compounds


				Ovalue	
21) Isophorone	9.40	82	12791	1.077	ng/ul# 75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA M\DATA\BM022318\
Data File : BM014331.D
Acq On : 23 Feb 2018 15:20
Operator : SJ/JU
Sample : PB106764BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Feb 23 15:52:17 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 22 03:35:18 2018
Response via : Initial Calibration

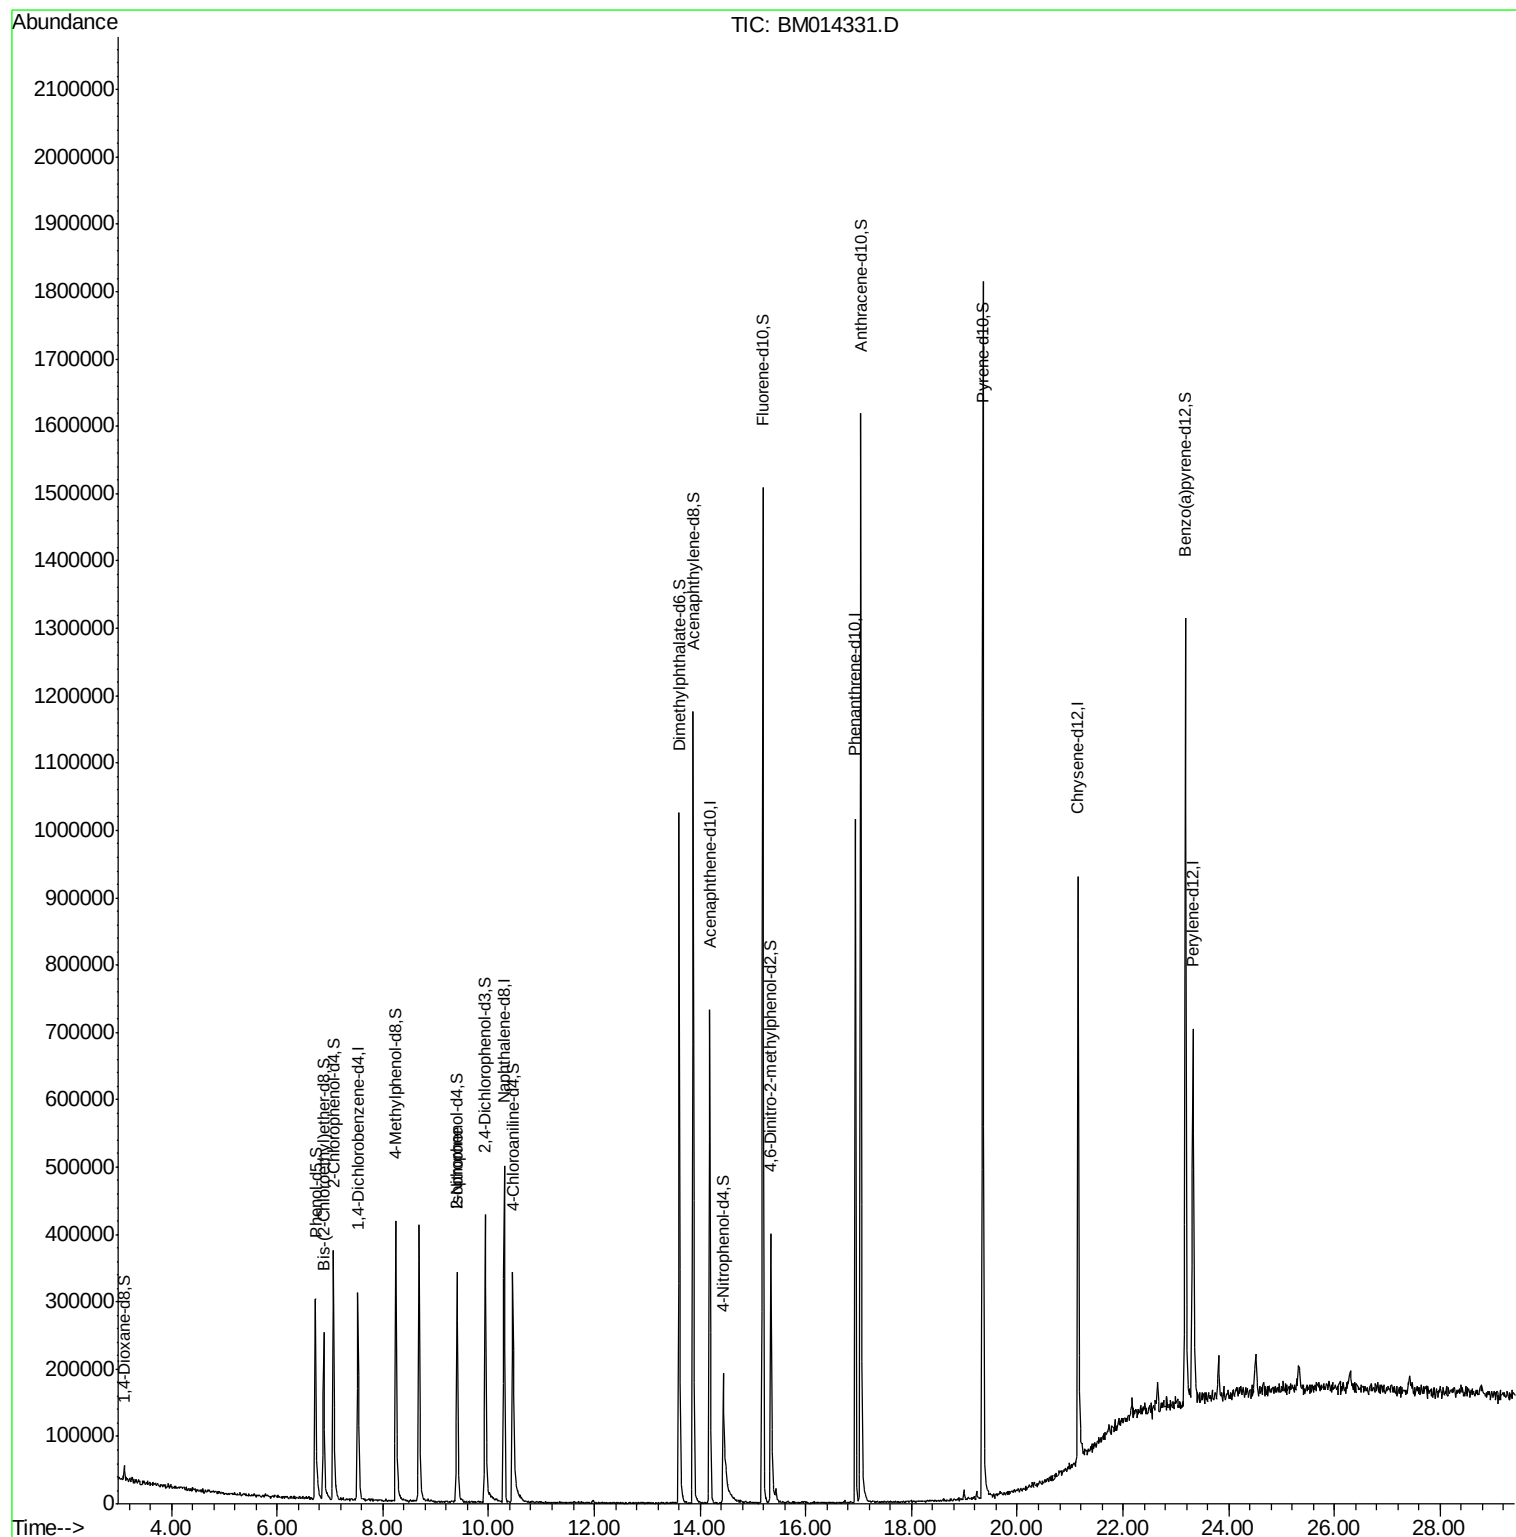

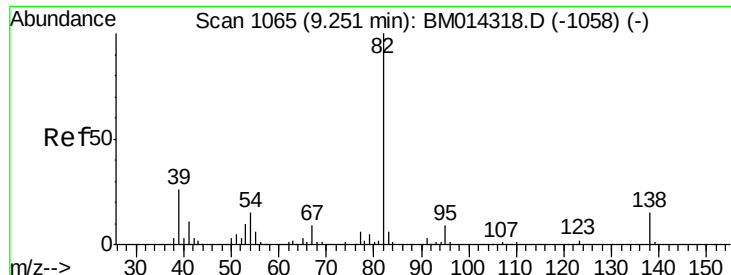

#21

Isophorone

Concen: 1.077 ng/ul

RT: 9.40 min Scan# 1090

Delta R.T. 0.15 min

Lab File: BM014331.D

Acq: 23 Feb 2018 15:20

Instrument :

BNA_M

ClientSampleId :

Tot Ion: 82 Resp: 12791

Ion Ratio Lower Upper

82 100

95 6.5 7.8 11.8#

138 0.0 11.9 17.9#

