

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022318\
 Data File : BM014345.D
 Acq On : 23 Feb 2018 23:43
 Operator : SJ/JU
 Sample : J1631-09 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BE5Z0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM021418.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.734	631	637	650	rBV6	32532	111122	4.50%	0.554%
2	6.887	658	663	667	rBV2	34823	60905	2.47%	0.304%
3	7.069	690	694	706	rBV4	50940	94278	3.82%	0.470%
4	7.528	765	772	784	rBV	520030	941077	38.09%	4.692%
5	8.263	887	897	903	rBV4	42095	86941	3.52%	0.433%
6	8.698	966	971	981	rBV2	45846	109930	4.45%	0.548%
7	9.410	1088	1092	1100	rBV3	38719	79063	3.20%	0.394%
8	9.975	1182	1188	1193	rBV6	29714	74790	3.03%	0.373%
9	10.292	1235	1242	1258	rBV	786108	1445644	58.52%	7.208%
10	13.604	1801	1805	1810	rBV	129857	206623	8.36%	1.030%
11	13.657	1810	1814	1825	rVB3	64320	122880	4.97%	0.613%
12	13.874	1845	1851	1861	rVB	184035	286954	11.62%	1.431%
13	14.180	1896	1903	1911	rBV2	1209849	1829537	74.06%	9.122%
14	14.245	1911	1914	1920	rVB5	19218	32289	1.31%	0.161%
15	15.186	2067	2074	2081	rBV2	190969	324489	13.13%	1.618%
16	15.245	2081	2084	2093	rVB4	19951	34730	1.41%	0.173%
17	15.362	2097	2104	2110	rBV6	24159	43581	1.76%	0.217%
18	16.257	2248	2256	2261	rBV6	9606	25469	1.03%	0.127%
19	16.609	2311	2316	2321	rBV5	14636	28618	1.16%	0.143%
20	16.756	2339	2341	2352	rVB4	23704	42261	1.71%	0.211%
21	16.939	2366	2372	2376	rBV	1433977	2017197	81.65%	10.057%
22	16.980	2376	2379	2385	rVB	328266	465465	18.84%	2.321%
23	17.045	2385	2390	2393	rBV2	200865	313590	12.69%	1.564%
24	17.368	2441	2445	2449	rBV	25008	35616	1.44%	0.178%
25	17.815	2516	2521	2524	rBV2	51062	84484	3.42%	0.421%
26	17.868	2524	2530	2535	rVB6	74060	161096	6.52%	0.803%
27	17.951	2540	2544	2548	rVV6	24777	45019	1.82%	0.224%
28	18.009	2550	2554	2558	rVV2	82709	143835	5.82%	0.717%
29	18.051	2558	2561	2569	rVB4	42849	67763	2.74%	0.338%
30	18.221	2587	2590	2596	rVB8	17675	30148	1.22%	0.150%
31	18.333	2604	2609	2613	rBV3	33315	57476	2.33%	0.287%
32	18.386	2615	2618	2623	rVB7	27996	47911	1.94%	0.239%
33	18.568	2641	2649	2655	rBV7	29437	86172	3.49%	0.430%
34	18.745	2675	2679	2681	rBV4	42741	61563	2.49%	0.307%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022318\
Data File : BM014345.D
Acq On : 23 Feb 2018 23:43
Operator : SJ/JU
Sample : J1631-09 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE5Z0

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM021418.M
Title : SVOA CALIBRATION

35	18.780	2681	2685	2688	rVV6	70836	90233	3.65%	0.450%
36	18.898	2700	2705	2710	rBV6	44980	87190	3.53%	0.435%
37	19.009	2718	2724	2731	rBV	748199	1047470	42.40%	5.222%
38	19.068	2731	2734	2736	rVV4	26458	29453	1.19%	0.147%
39	19.127	2740	2744	2748	rBV6	30151	59421	2.41%	0.296%
40	19.250	2763	2765	2769	rVB4	36847	37911	1.53%	0.189%
41	19.345	2776	2781	2783	rBV	363819	516575	20.91%	2.576%
42	19.374	2783	2786	2796	rVB	872114	1225932	49.62%	6.112%
43	19.456	2797	2800	2803	rVV4	32580	36254	1.47%	0.181%
44	19.709	2839	2843	2850	rVB7	55075	108515	4.39%	0.541%
45	19.874	2869	2871	2877	rVB2	98278	131110	5.31%	0.654%
46	19.980	2886	2889	2893	rBV2	57406	68631	2.78%	0.342%
47	20.039	2895	2899	2904	rVB3	79873	127183	5.15%	0.634%
48	20.174	2920	2922	2926	rVB3	49098	54293	2.20%	0.271%
49	20.221	2927	2930	2935	rVB	58817	75477	3.06%	0.376%
50	20.639	2999	3001	3006	rVB2	76075	84923	3.44%	0.423%
51	20.797	3025	3028	3031	rBV2	69294	83229	3.37%	0.415%
52	20.833	3031	3034	3037	rVV2	78234	89716	3.63%	0.447%
53	20.874	3038	3041	3046	rVB2	97622	150141	6.08%	0.749%
54	21.150	3081	3088	3092	rBV2	1515375	2470466	100.00%	12.317%
55	21.186	3092	3094	3099	rVB	385686	409595	16.58%	2.042%
56	21.303	3111	3114	3117	rVB3	98750	97843	3.96%	0.488%
57	22.674	3342	3347	3353	rBV	440053	1005172	40.69%	5.012%
58	23.133	3421	3425	3429	rBV	237571	363294	14.71%	1.811%
59	23.227	3437	3441	3449	rVB	367928	662986	26.84%	3.306%
60	23.321	3451	3457	3462	rBV	743322	1345343	54.46%	6.708%


Sum of corrected areas: 20056872

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022318\
Data File : BM014345.D
Acq On : 23 Feb 2018 23:43
Operator : SJ/JU
Sample : J1631-09 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE5Z0

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

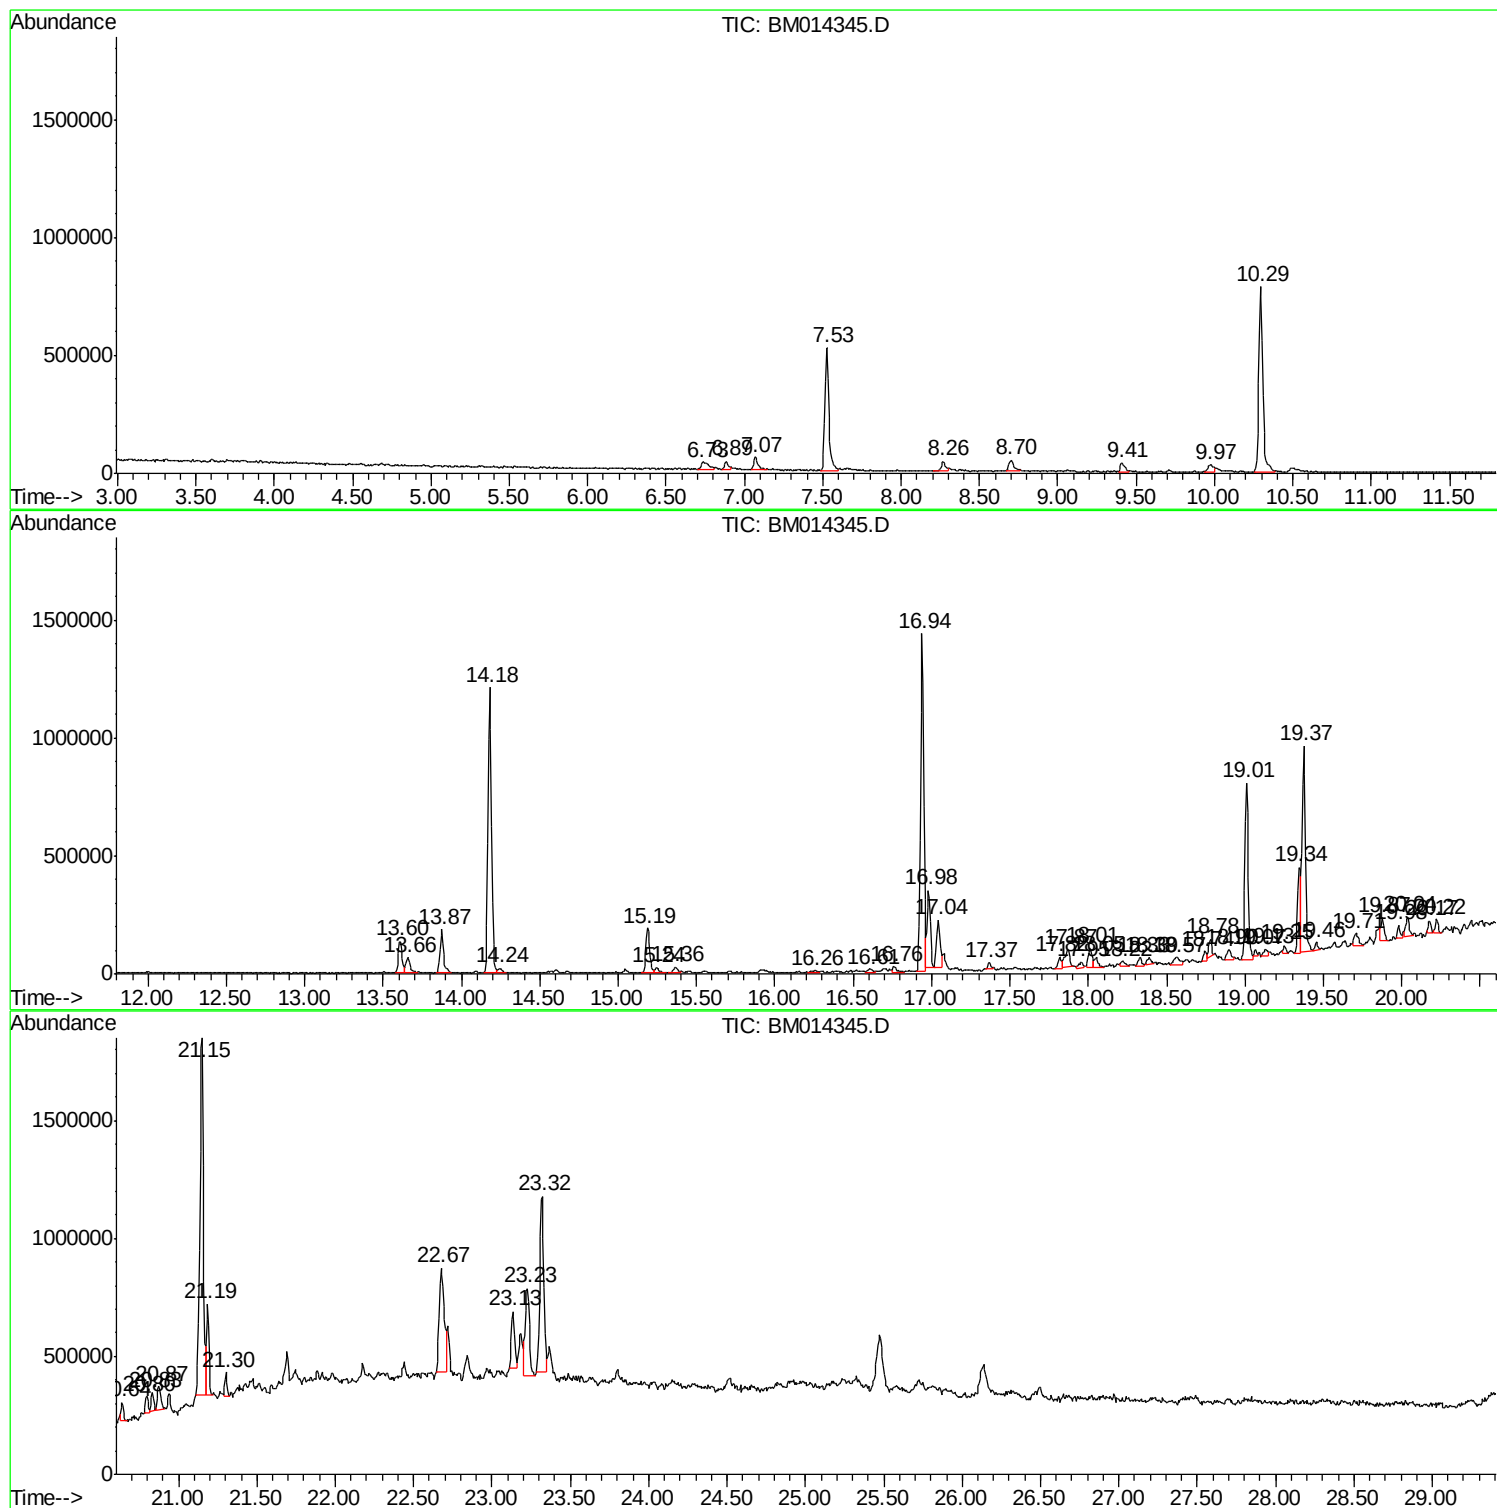

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022318\
Data File : BM014345.D
Acq On : 23 Feb 2018 23:43
Operator : SJ/JU
Sample : J1631-09 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE5Z0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022318\
Data File : BM014345.D
Acq On : 23 Feb 2018 23:43
Operator : SJ/JU
Sample : J1631-09 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE5Z0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc