

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022321\
 Data File : BM028875.D
 Acq On : 23 Feb 2021 17:12
 Operator : CG/JU
 Sample : PB134764BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB134764BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM028875.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.363	398	404	416	rBV	379528	524898	65.33%	12.150%
2	6.998	675	682	698	rBB	341436	524984	65.34%	12.152%
3	7.804	814	819	827	rBB	68040	103611	12.90%	2.398%
4	8.986	1013	1020	1029	rBV	209793	330547	41.14%	7.651%
5	10.610	1290	1296	1304	rBB	87870	139613	17.38%	3.232%
6	13.086	1710	1717	1725	rBB	516903	711992	88.62%	16.481%
7	14.468	1946	1952	1958	rBB2	123541	172684	21.49%	3.997%
8	15.962	2200	2206	2213	rBB	380534	495469	61.67%	11.469%
9	17.209	2412	2418	2424	rBV	136177	181407	22.58%	4.199%
10	19.827	2857	2863	2868	rBV	671063	803466	100.00%	18.598%
11	21.374	3121	3126	3130	rBV	137108	170250	21.19%	3.941%
12	23.586	3496	3502	3510	rBV	92163	161145	20.06%	3.730%




Sum of corrected areas: 4320066

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022321\
Data File : BM028875.D
Acq On : 23 Feb 2021 17:12
Operator : CG/JU
Sample : PB134764BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB134764BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

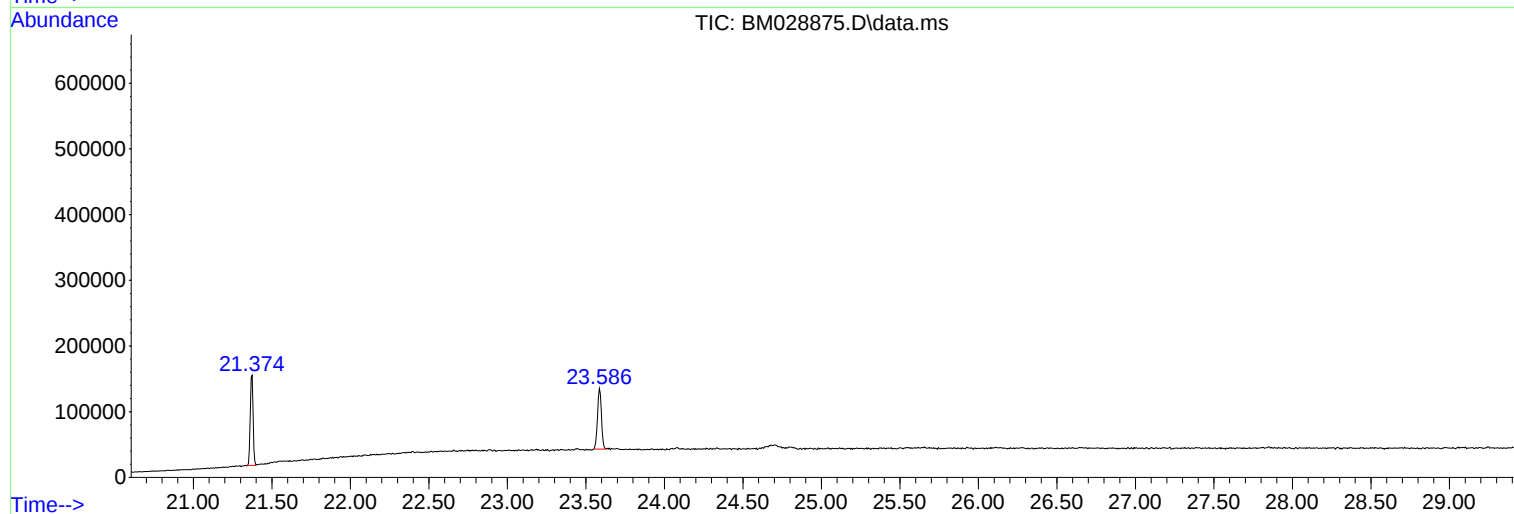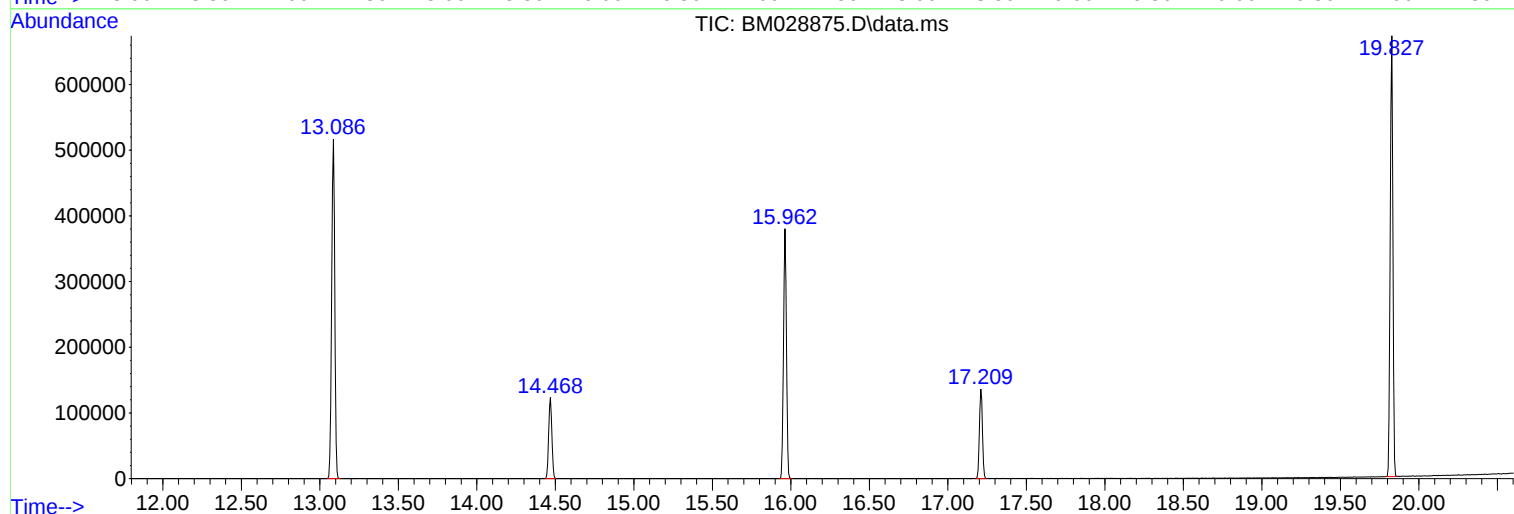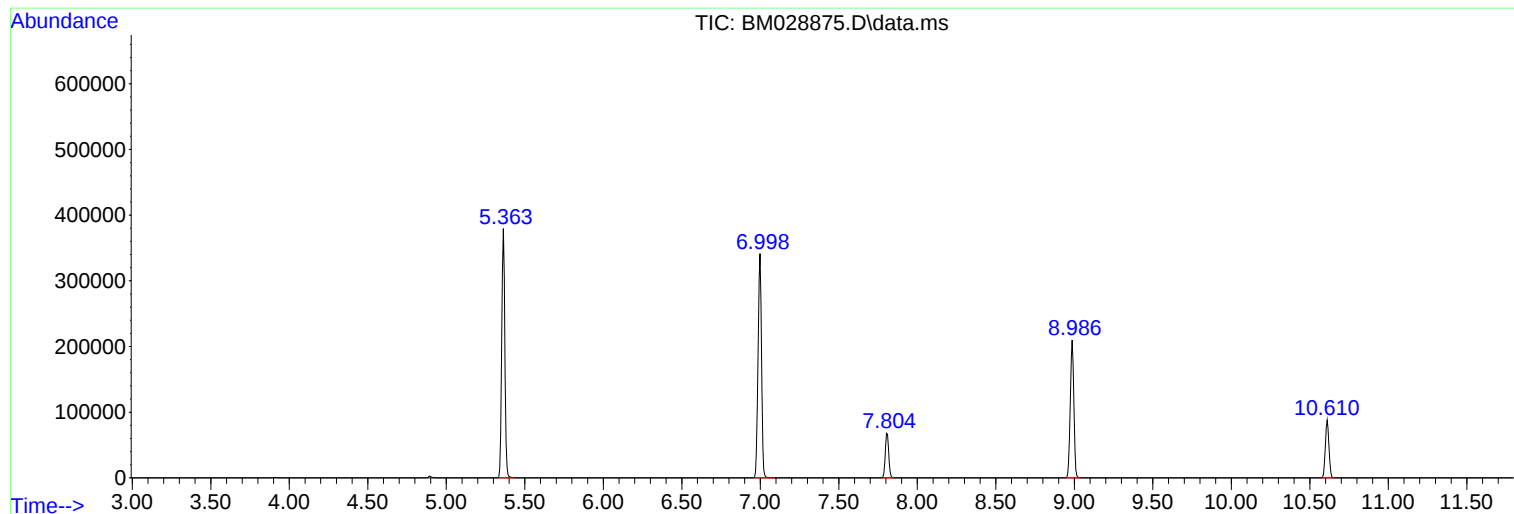

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022321\
Data File : BM028875.D
Acq On : 23 Feb 2021 17:12
Operator : CG/JU
Sample : PB134764BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB134764BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022321\
Data File : BM028875.D
Acq On : 23 Feb 2021 17:12
Operator : CG/JU
Sample : PB134764BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB134764BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------