


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022321\
 Data File : BM028866.D
 Acq On : 23 Feb 2021 10:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 23 16:39:41 2021

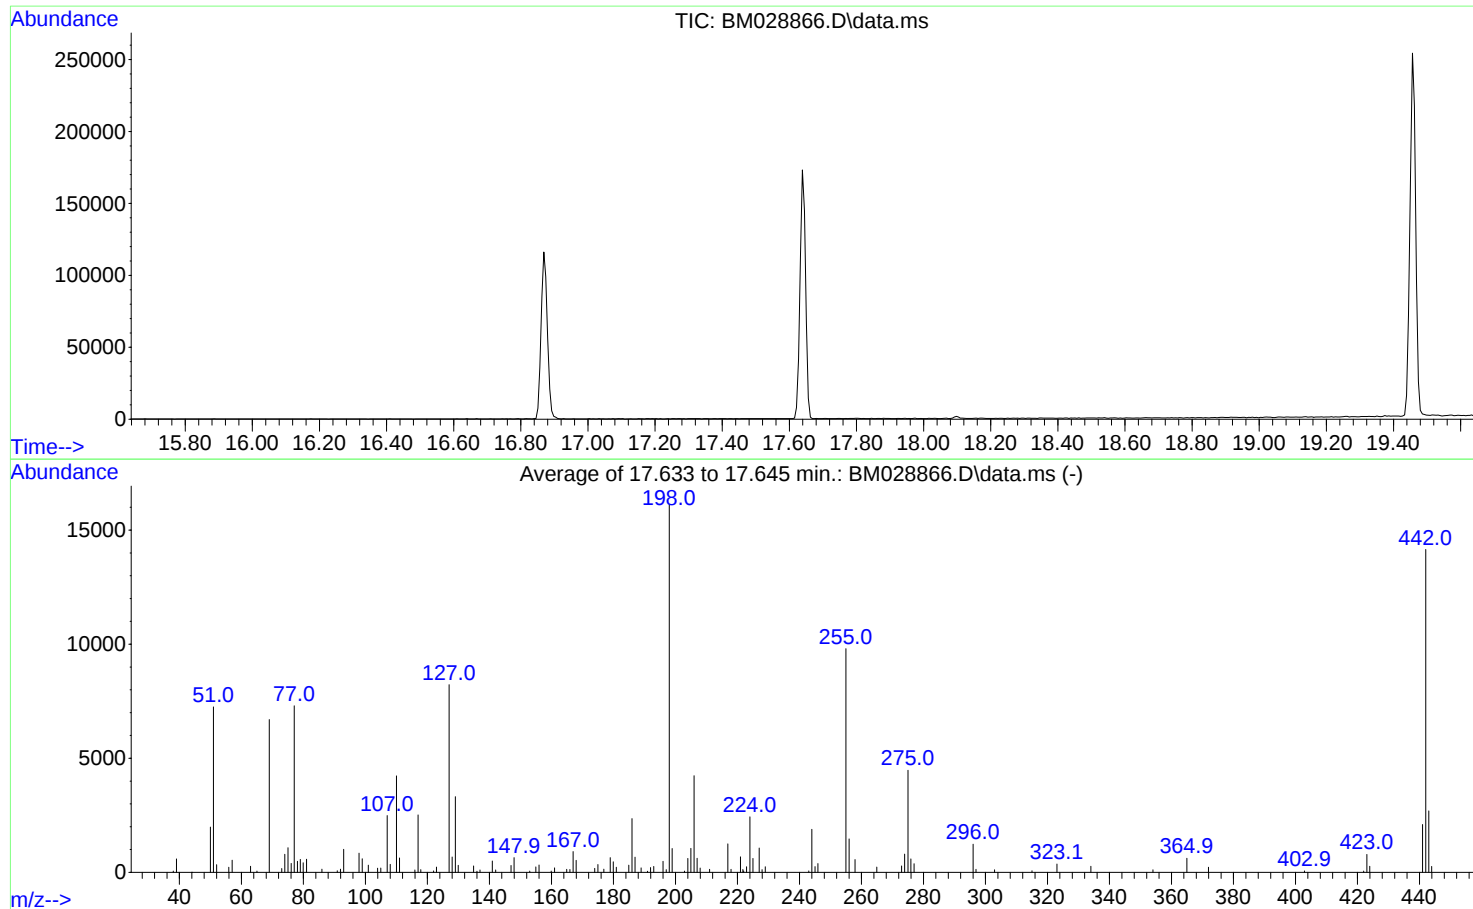

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.0	7252	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	41.5	6697	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.0	8227	PASS
197	198	0.00	2	0.8	122	PASS
198	198	100	100	100.0	16122	PASS
199	198	5	9	6.5	1048	PASS
275	198	10	60	27.7	4471	PASS
365	198	1	100	3.8	619	PASS
441	198	0.01	100	13.0	2097	PASS
442	442	50	100	100.0	14153	PASS
443	442	15	24	19.0	2691	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/23/2021	BNA_M	<u>BM028866.D</u>
Compound Name	Response	Retention Time
DDT	57652	20.674
DDD	114	20.286
DDE	0	19.821
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
114	57766	0.20

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022321\
Data File : BM028866.D
Acq On : 23 Feb 2021 10:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 23 18:09:11 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 23 16:39:41 2021
Response via : Initial Calibration

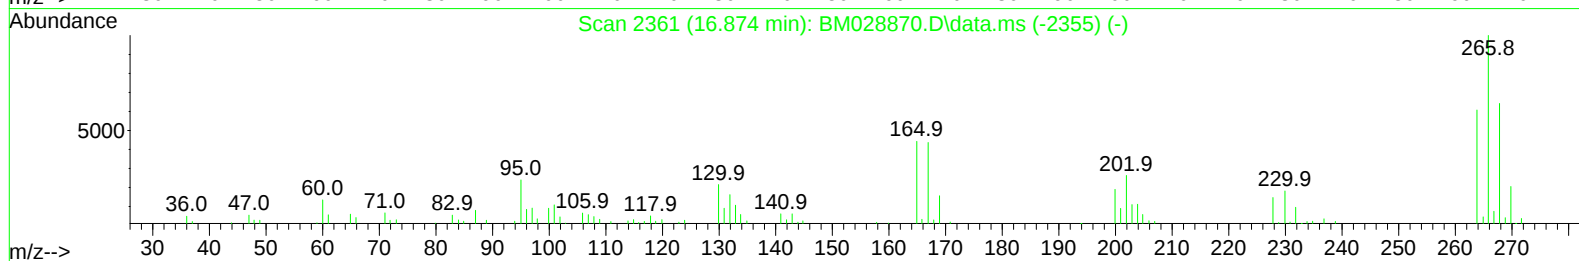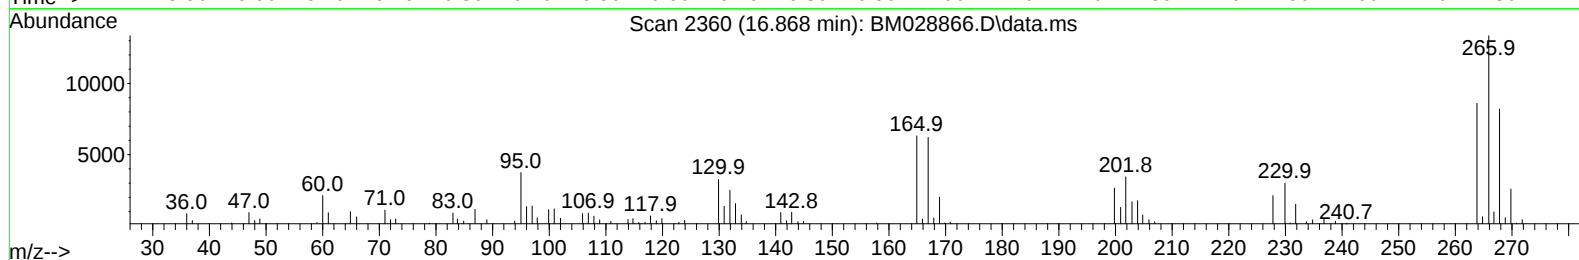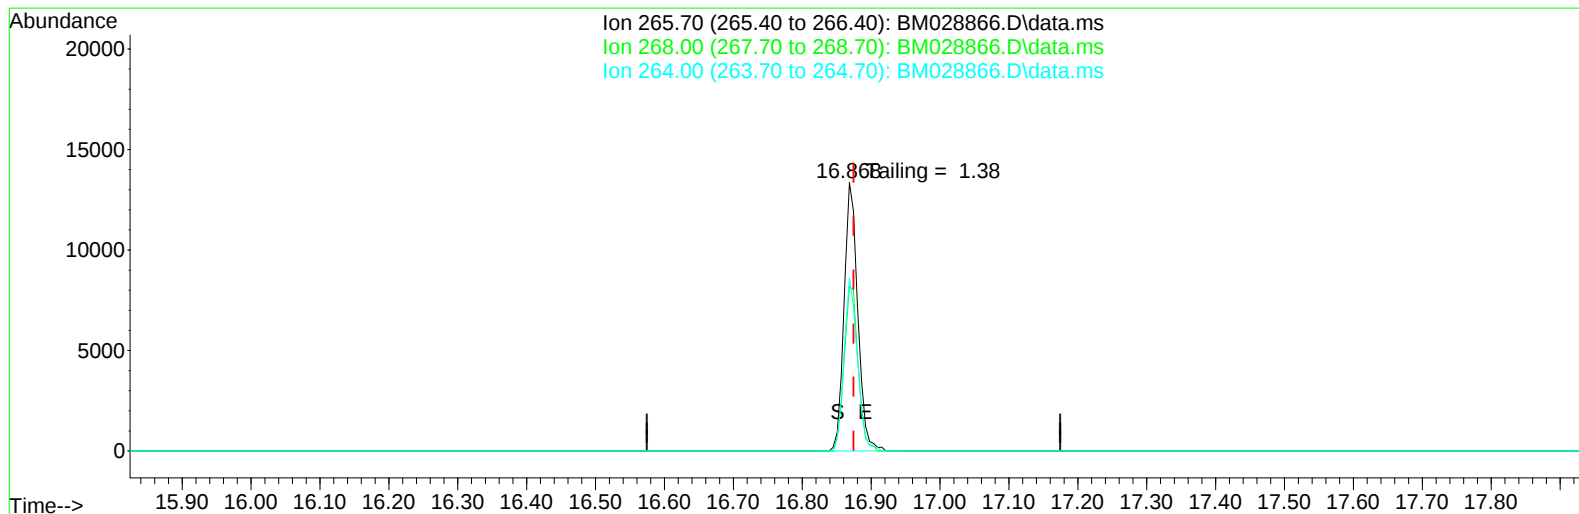

TIC: BM028866.D\data.ms

(70) Pentachlorophenol (C)

16.868min (-0.006) 0.00 ng




response 18499

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	61.49
264.00	63.30	64.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022321\
Data File : BM028866.D
Acq On : 23 Feb 2021 10:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 23 18:09:11 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 23 16:39:41 2021
Response via : Initial Calibration

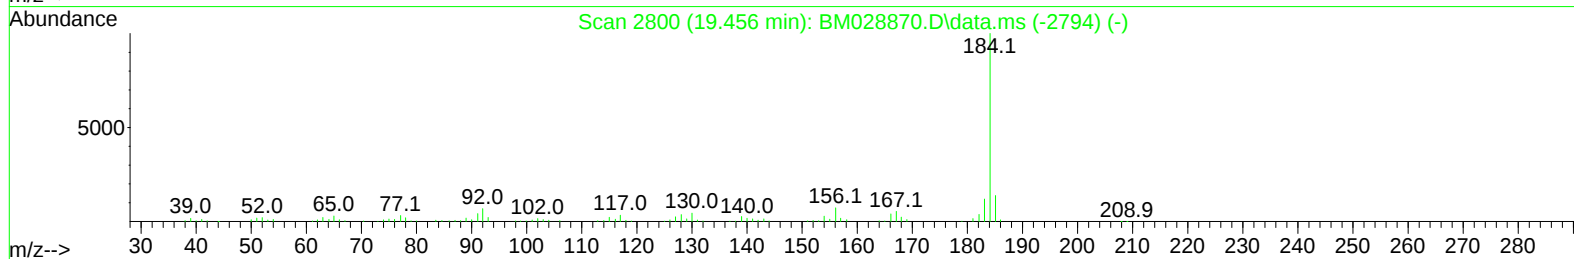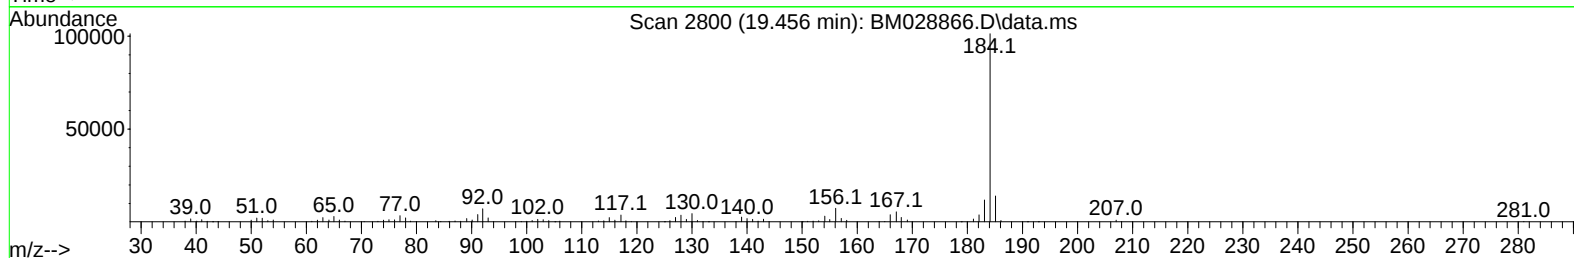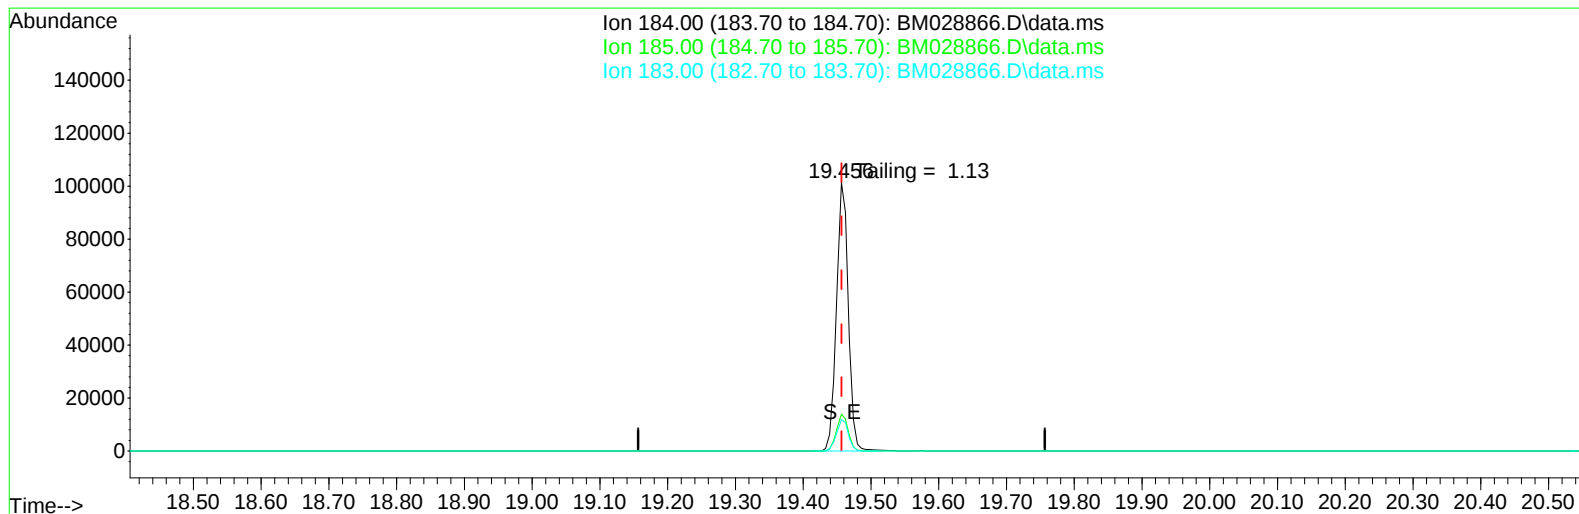

TIC: BM028866.D\data.ms

(77) Benzidine

19.456min (-0.000) 0.00 ng

response 123826

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	13.82
183.00	12.10	11.68
0.00	0.00	0.00