

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022324\
 Data File : BM044273.D
 Acq On : 23 Feb 2024 16:22
 Operator : MA/JU
 Sample : P1498-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB2

Quant Time: Feb 23 23:27:07 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 23 22:49:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.904	152	216626	20.000	ng/u1	0.01
20) Naphthalene-d8	10.704	136	902697	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.545	164	496886	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.298	188	1008041	20.000	ng/u1	0.00
79) Chrysene-d12	21.503	240	916737	20.000	ng/u1	0.00
88) Perylene-d12	23.903	264	1034267	20.000	ng/u1	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	31272	4.555	ng/uL	0.00
4) Pyridine-d5	3.763	84	277632	14.806	ng/u1	0.00
7) Phenol-d5	7.069	99	174509	8.409	ng/u1	0.01
9) Bis-(2-Chloroethyl)eth...	7.246	67	521564	38.812	ng/u1	0.00
11) 2-Chlorophenol-d4	7.428	132	480925	30.770	ng/u1	0.00
15) 4-Methylphenol-d8	8.616	113	94971	6.048	ng/u1	0.01
21) Nitrobenzene-d5	9.069	128	301155	41.031	ng/u1	0.00
24) 2-Nitrophenol-d4	9.792	143	309585	41.343	ng/u1	0.01
28) 2,4-Dichlorophenol-d3	10.328	165	432321	32.729	ng/u1	0.01
31) 4-Chloroaniline-d4	10.857	131	143529	6.470	ng/u1	0.01
46) Dimethylphthalate-d6	13.969	166	1621314	42.308	ng/u1	0.00
49) Acenaphthylene-d8	14.239	160	1810644	41.066	ng/u1	0.00
54) 4-Nitrophenol-d4	14.757	143	50280	6.594	ng/u1	0.01
60) Fluorene-d10	15.545	176	1392469	42.930	ng/u1	0.01
65) 4,6-Dinitro-2-methylph...	15.663	200	216297	34.581	ng/u1	0.00
73) Anthracene-d10	17.398	188	1690177	35.164	ng/u1	0.00
81) Pyrene-d10	19.704	212	2496050	45.257	ng/u1	0.01
92) Benzo(a)pyrene-d12	23.750	264	1906535	35.974	ng/u1	0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.439	149	68073	1.427	ng/u1#	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022324\
Data File : BM044273.D
Acq On : 23 Feb 2024 16:22
Operator : MA/JU
Sample : P1498-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB2


Quant Time: Feb 23 23:27:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 23 22:49:27 2024
Response via : Initial Calibration

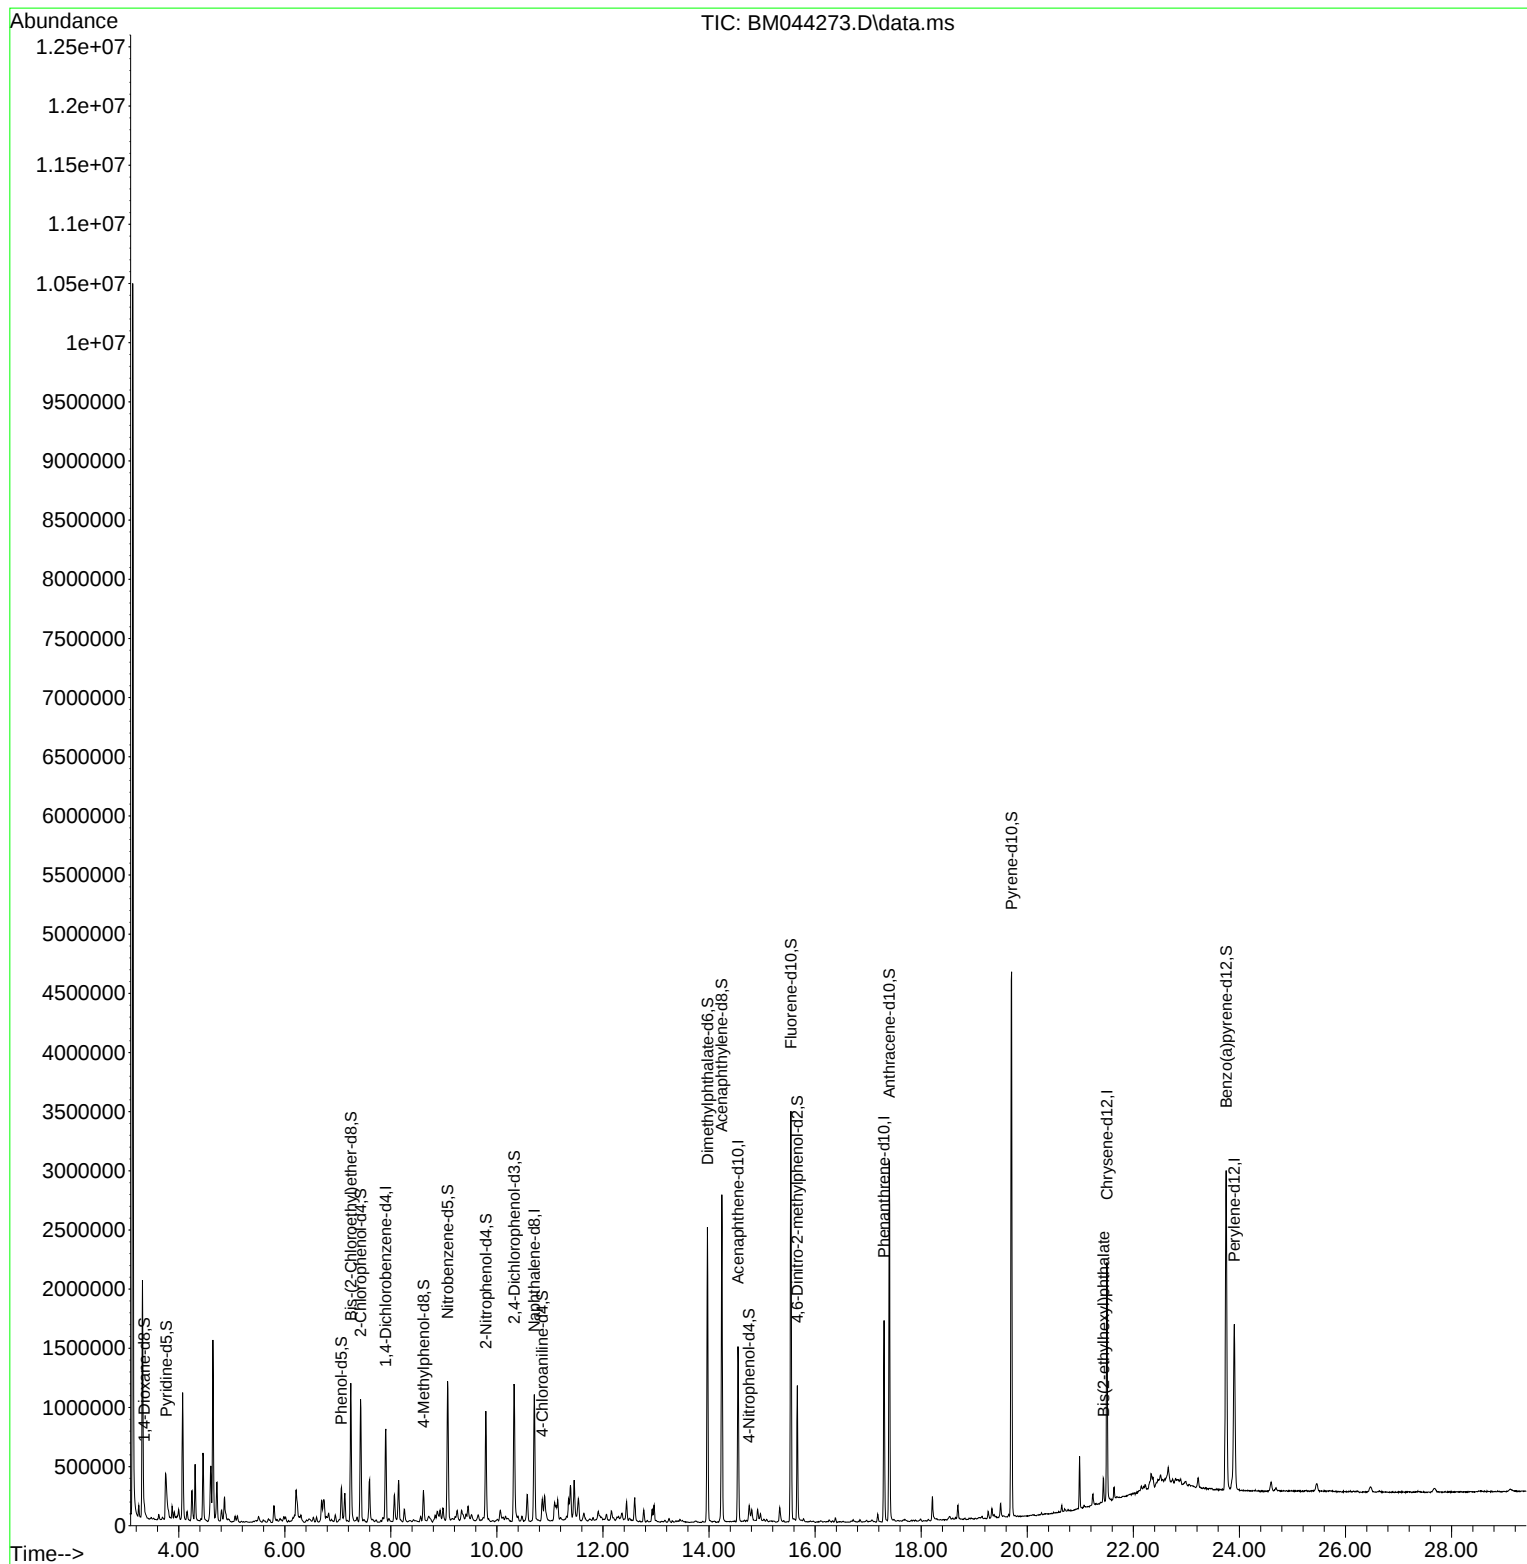

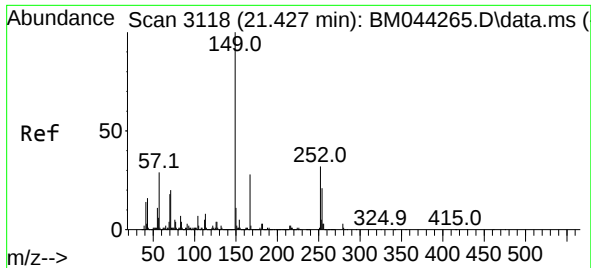

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.427 ng/ul
 RT: 21.439 min Scan# 31
 Delta R.T. 0.012 min
 Lab File: BM044273.D
 Acq: 23 Feb 2024 16:22

Instrument :
 BNA_M
 ClientSampleId :
 C0AB2

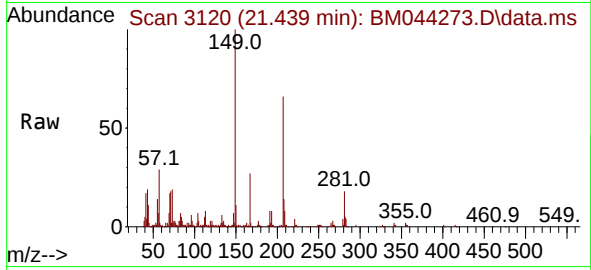

Tgt Ion:	149	Resp:	68073
Ion Ratio	Lower	Upper	
149	100		
167	27.5	22.1	33.1
279	3.9	2.4	3.6#

