

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022324\
 Data File : BM044274.D
 Acq On : 23 Feb 2024 16:59
 Operator : MA/JU
 Sample : P1498-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB3

Quant Time: Feb 23 23:14:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 23 22:49:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.904	152	188390	20.000	ng/u1	0.01
20) Naphthalene-d8	10.704	136	794949	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.545	164	441622	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.298	188	904247	20.000	ng/u1	0.00
79) Chrysene-d12	21.503	240	811094	20.000	ng/u1	0.00
88) Perylene-d12	23.903	264	899893	20.000	ng/u1	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.351	96	29396	4.923	ng/uL	0.00
4) Pyridine-d5	3.763	84	325798	19.979	ng/u1	0.00
7) Phenol-d5	7.069	99	158685	8.793	ng/u1	0.01
9) Bis-(2-Chloroethyl)eth...	7.245	67	477419	40.851	ng/u1	0.00
11) 2-Chlorophenol-d4	7.428	132	433187	31.870	ng/u1	0.00
15) 4-Methylphenol-d8	8.616	113	53445	3.914	ng/u1	0.01
21) Nitrobenzene-d5	9.075	128	278629	43.108	ng/u1	0.01
24) 2-Nitrophenol-d4	9.792	143	287869	43.653	ng/u1	0.01
28) 2,4-Dichlorophenol-d3	10.327	165	387549	33.316	ng/u1	0.01
31) 4-Chloroaniline-d4	10.857	131	137360	7.031	ng/u1	0.01
46) Dimethylphthalate-d6	13.968	166	1584639	46.525	ng/u1	0.00
49) Acenaphthylene-d8	14.239	160	1748917	44.630	ng/u1	0.00
54) 4-Nitrophenol-d4	14.757	143	49323	7.277	ng/u1	0.01
60) Fluorene-d10	15.545	176	1355515	47.021	ng/u1	0.01
65) 4,6-Dinitro-2-methylph...	15.662	200	211743	37.739	ng/u1	0.00
73) Anthracene-d10	17.398	188	1612235	37.393	ng/u1	0.00
81) Pyrene-d10	19.703	212	2352800	48.217	ng/u1	0.01
92) Benzo(a)pyrene-d12	23.750	264	1744437	37.831	ng/u1	0.01


Target Compounds					Qvalue
86) Bis(2-ethylhexyl)phtha...	21.438	149	64638	1.532 ng/u1#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022324\
Data File : BM044274.D
Acq On : 23 Feb 2024 16:59
Operator : MA/JU
Sample : P1498-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB3


Quant Time: Feb 23 23:14:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 23 22:49:27 2024
Response via : Initial Calibration

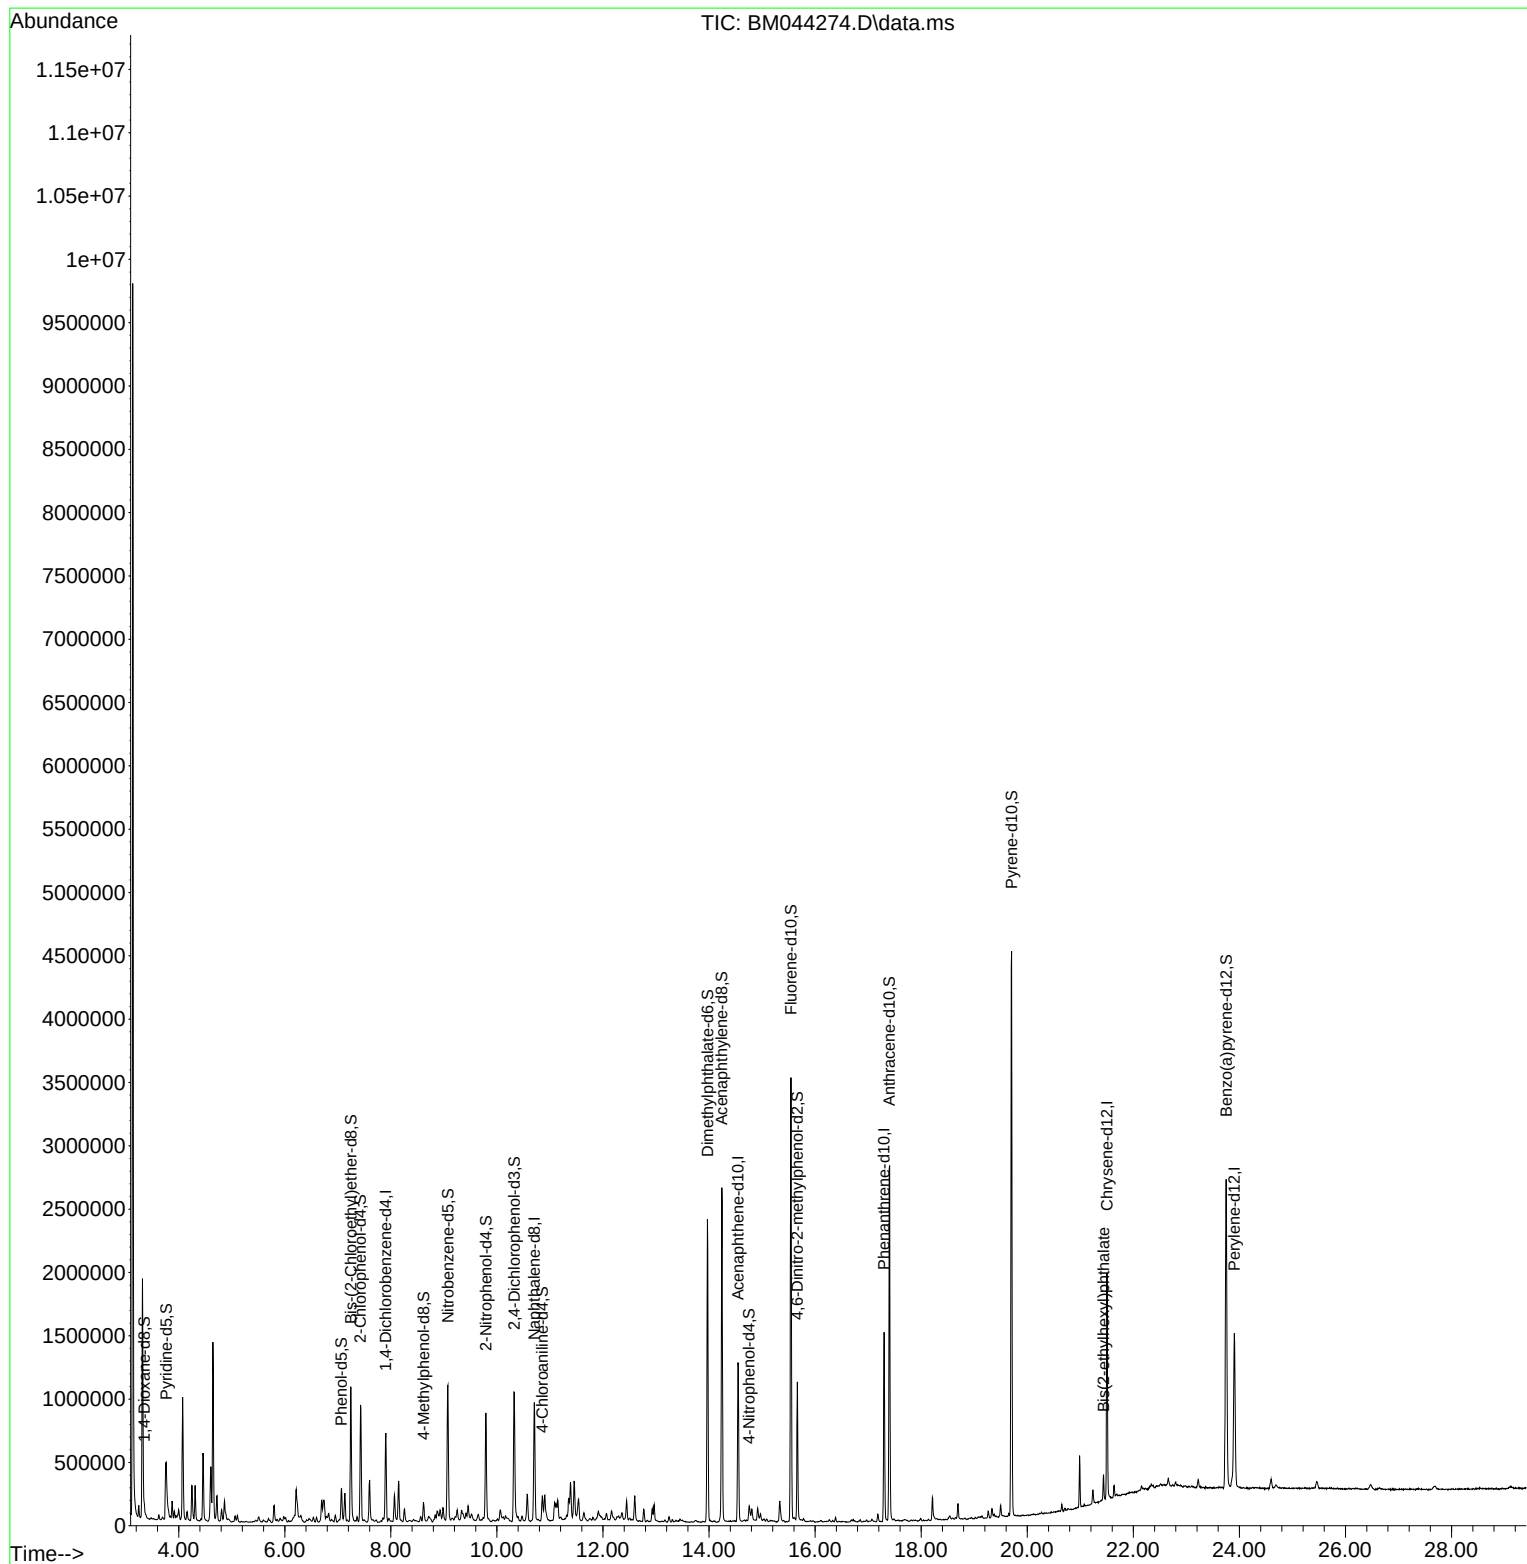

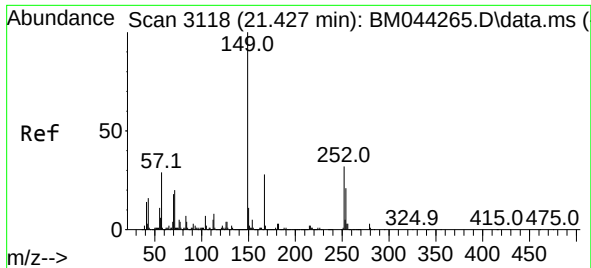

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.532 ng/ul
 RT: 21.438 min Scan# 31
 Delta R.T. 0.012 min
 Lab File: BM044274.D
 Acq: 23 Feb 2024 16:59

Instrument :
 BNA_M
 ClientSampleId :
 C0AB3

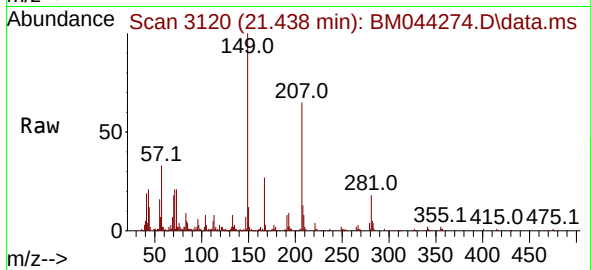

Tgt Ion:149 Resp: 64638
 Ion Ratio Lower Upper
 149 100
 167 26.6 22.1 33.1
 279 4.0 2.4 3.6#

