




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022416\
Data File : BM004394.D
Acq On : 24 Feb 2016 20:34
Operator : SJ/UM
Sample : H1515-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0311-S19-0312

Manual Integrations
APPROVED

UMANGI
2/25/2016 2:43:47 PM

Quant Time: Feb 25 02:18:21 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 25 02:09:59 2016
Response via : Initial Calibration

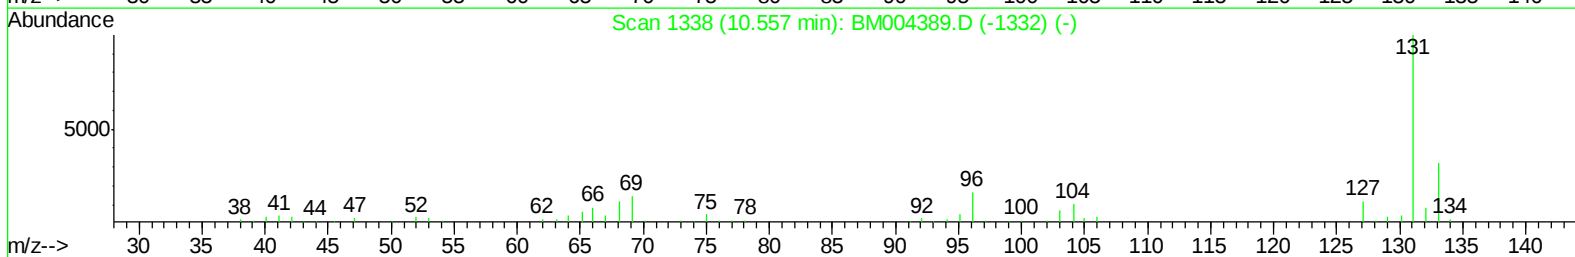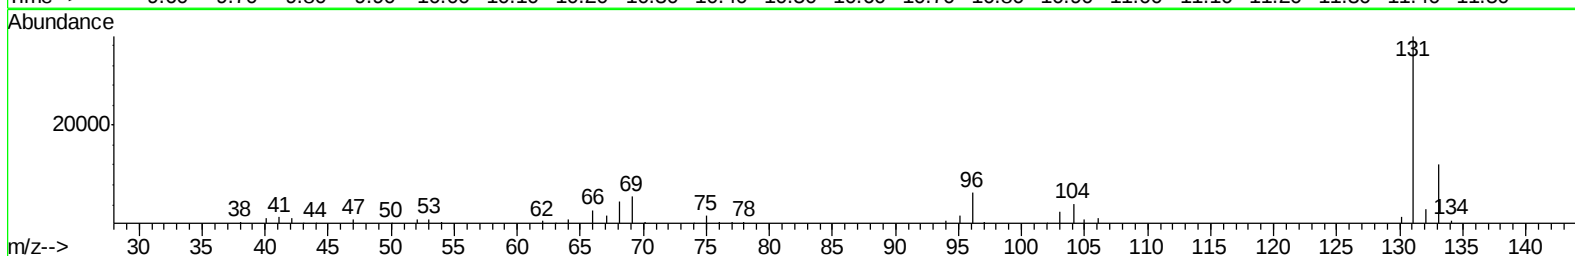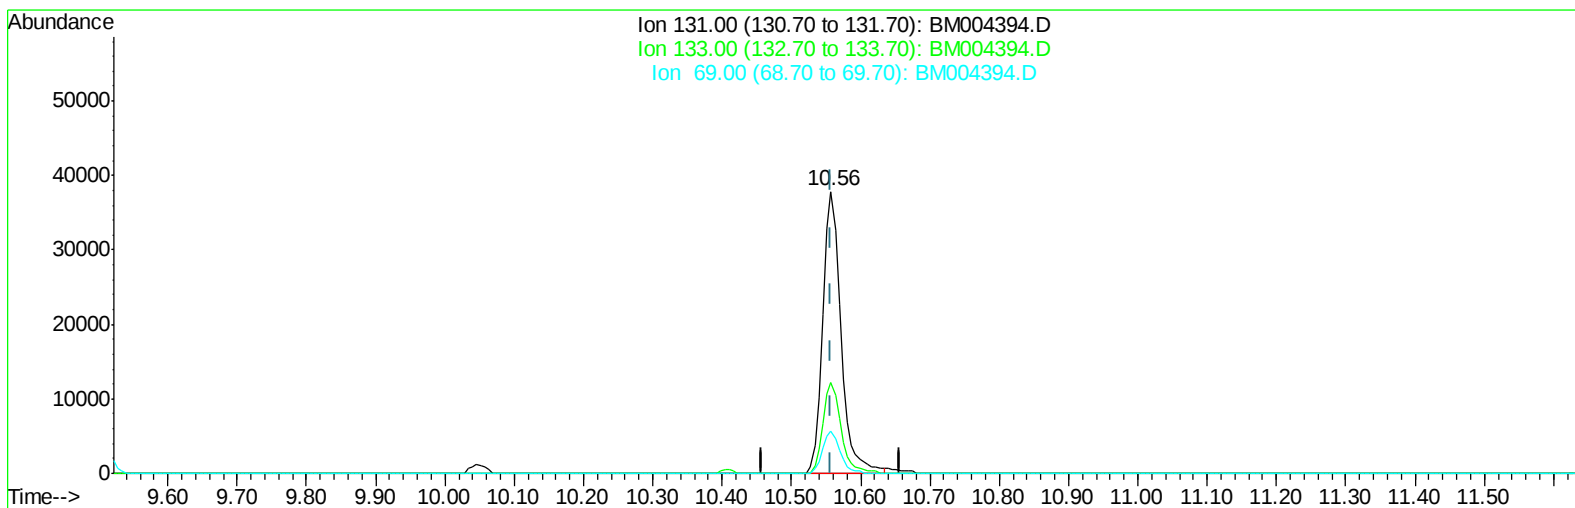

TIC: BM004394.D

(29) 4-Chloroaniline-d4 (S)
10.557min (+0.000) 30.20ng/ul
response 68970

Ion	Exp%	Act%
131.00	100	100
133.00	32.10	32.37
69.00	16.20	15.06
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022416\
Data File : BM004394.D
Acq On : 24 Feb 2016 20:34
Operator : SJ/UM
Sample : H1515-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0311-S19-0312

Manual Integrations
APPROVED

UMANGI
2/25/2016 2:43:47 PM

Quant Time: Feb 25 02:18:21 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 25 02:09:59 2016
Response via : Initial Calibration

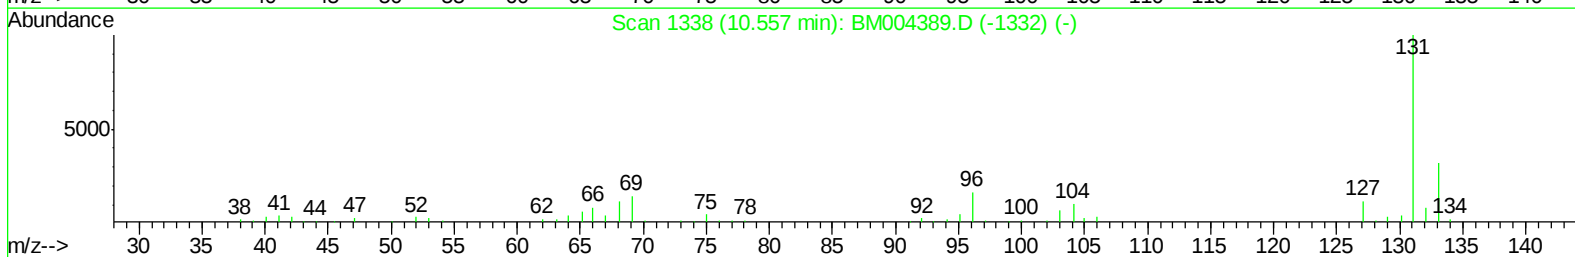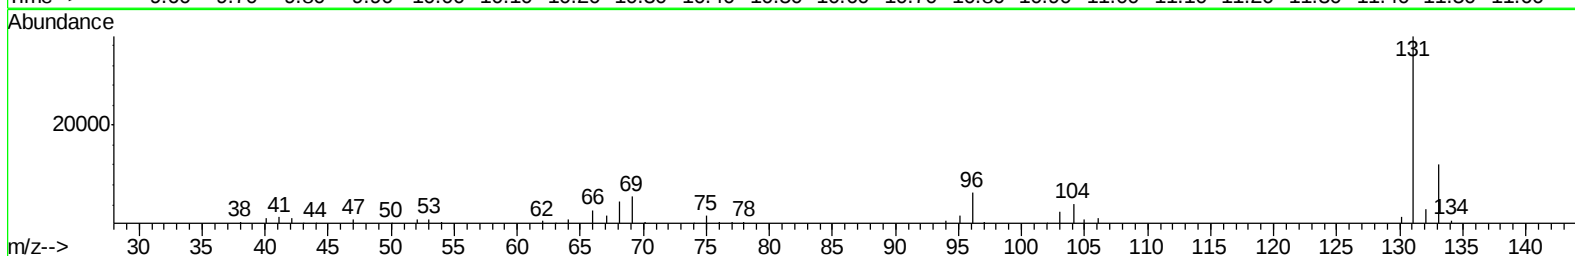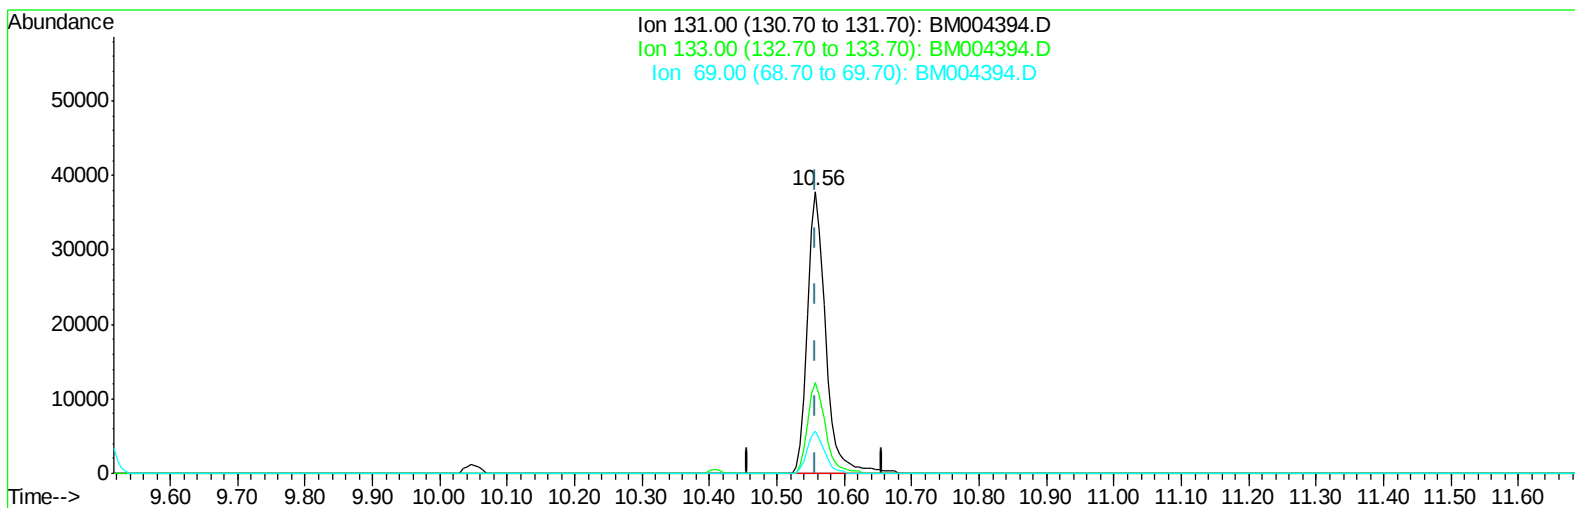

TIC: BM004394.D

(29) 4-Chloroaniline-d4 (S)

10.557min (+0.000) 30.69ng/ul m

response 70094

Ion	Exp%	Act%
131.00	100	100
133.00	32.10	32.37
69.00	16.20	15.06
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022416\
Data File : BM004394.D
Acq On : 24 Feb 2016 20:34
Operator : SJ/UM
Sample : H1515-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0311-S19-0312

Manual Integrations
APPROVED

UMANGI
2/25/2016 2:43:47 PM

Quant Time: Feb 25 02:18:21 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 25 02:09:59 2016
Response via : Initial Calibration

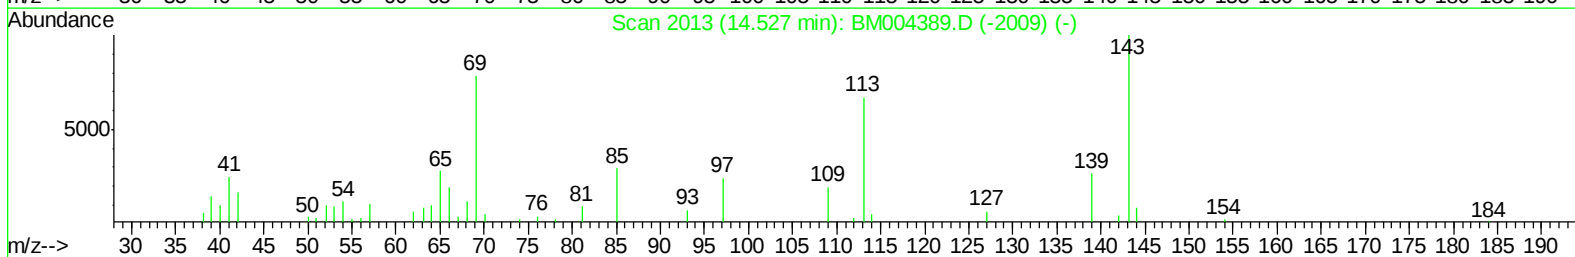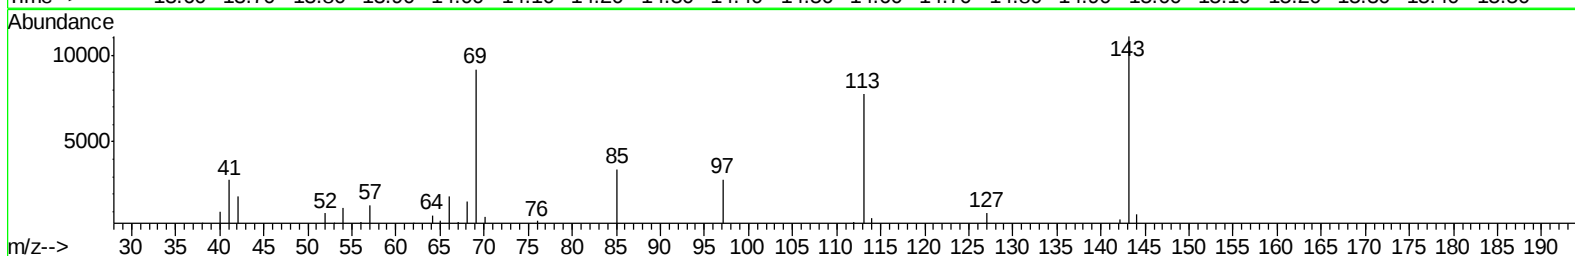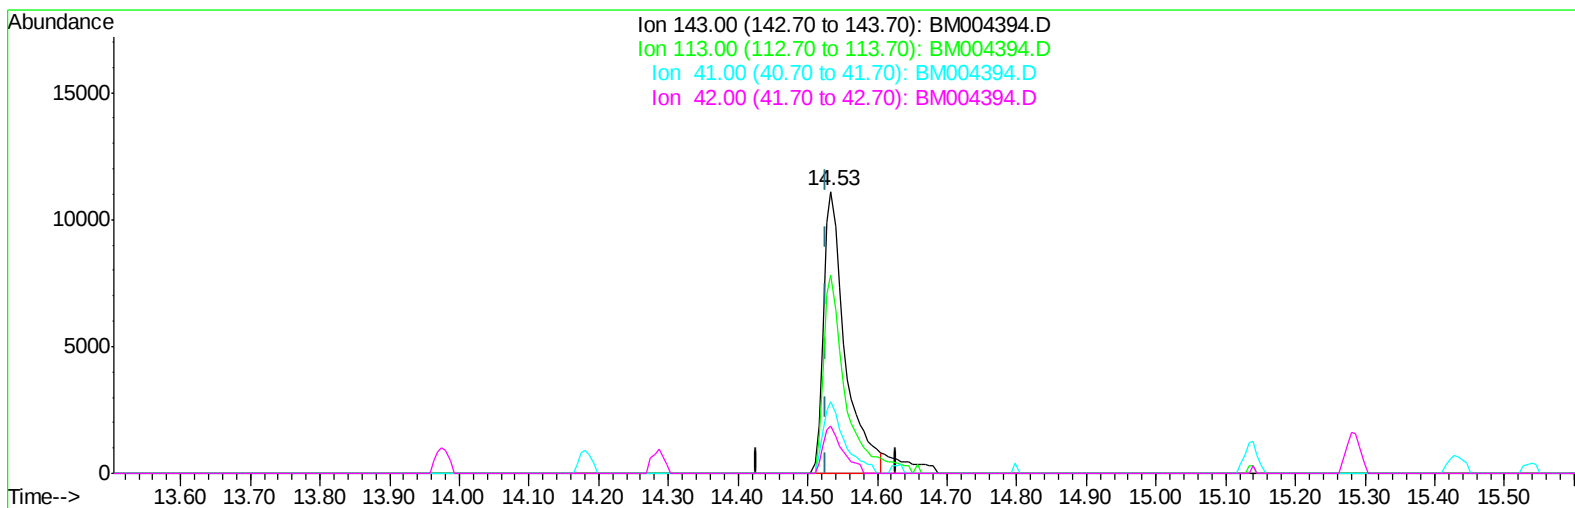

TIC: BM004394.D

(52) 4-Nitrophenol-d4 (S)

14.533min (+0.006) 23.45ng/ul

response 23848

Ion	Exp%	Act%
143.00	100	100
113.00	75.10	70.25
41.00	28.80	25.32
42.00	19.10	16.82




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022416\
Data File : BM004394.D
Acq On : 24 Feb 2016 20:34
Operator : SJ/UM
Sample : H1515-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0311-S19-0312

Manual Integrations
APPROVED

UMANGI
2/25/2016 2:43:47 PM

Quant Time: Feb 25 02:18:21 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 25 02:09:59 2016
Response via : Initial Calibration

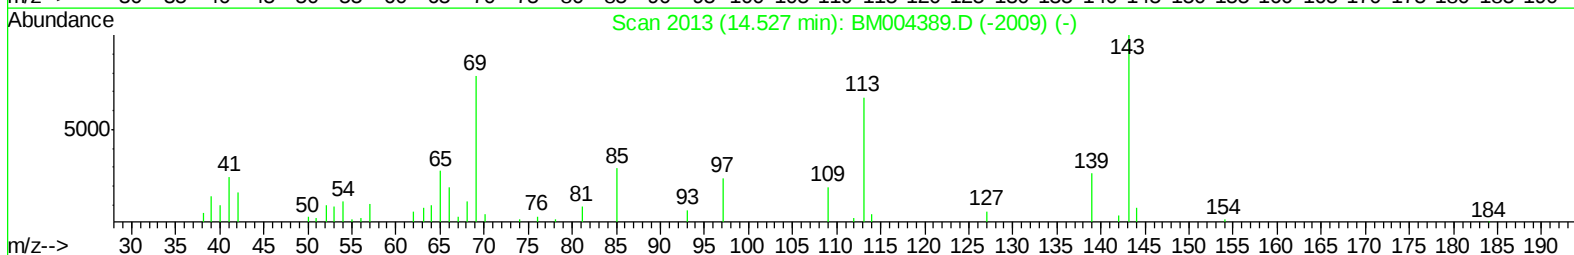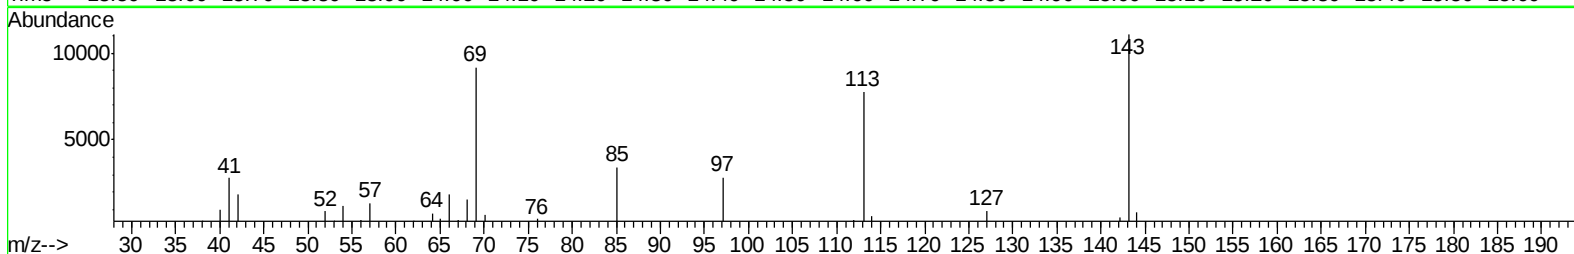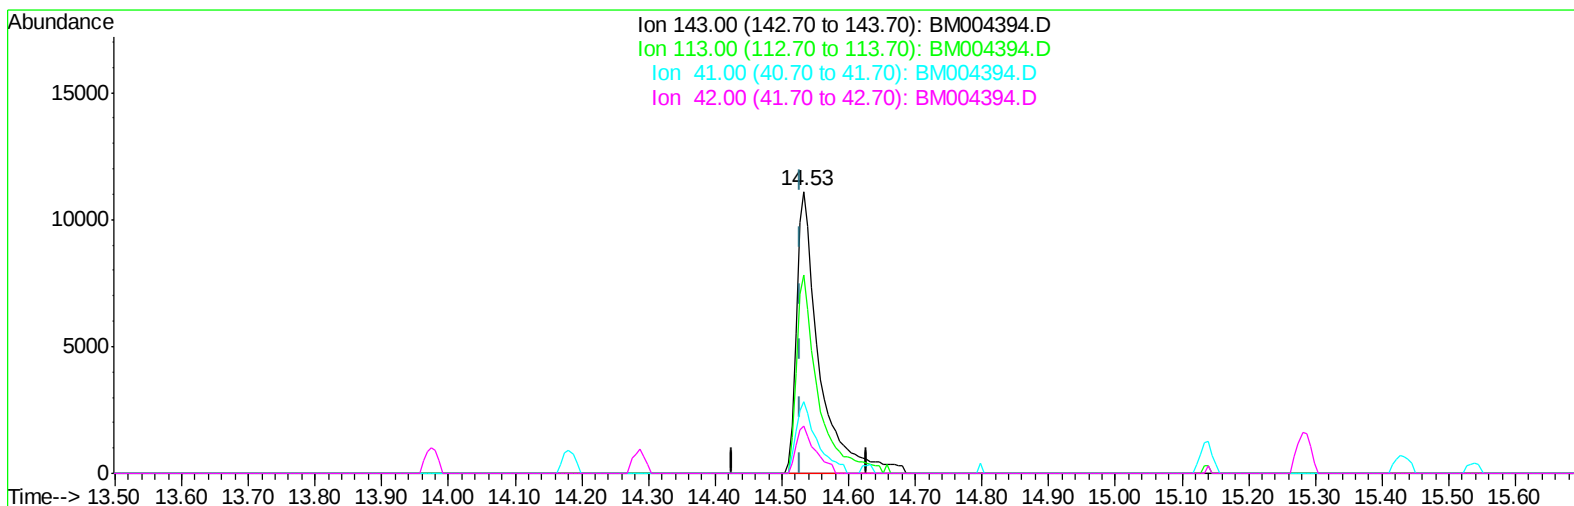

TIC: BM004394.D

(52) 4-Nitrophenol-d4 (S)

14.533min (+0.006) 25.53ng/ul m

response 25964

Ion	Exp%	Act%
143.00	100	100
113.00	75.10	70.25
41.00	28.80	25.32
42.00	19.10	16.82

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022416\
 Data File : BM004394.D
 Acq On : 24 Feb 2016 20:34
 Operator : SJ/UM
 Sample : H1515-14
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-S19-0312

Manual Integrations
 APPROVED

UMANGI
 2/25/2016 2:43:47 PM

Quant Time: Feb 25 02:49:02 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 25 02:09:59 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	23441	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	116899	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	73786	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	170317	20.00	ng/ul	0.00
78) Chrysene-d12	21.25	240	181681	20.00	ng/ul	0.00
86) Perylene-d12	23.47	264	135256	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.08	96	2299	5.17	ng/uL	0.00
5) Phenol-d5	6.81	99	57176	29.09	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	30094	30.10	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	51488	30.37	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	43200	24.60	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	26680	30.00	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	30810	30.39	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	54087	29.52	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	70094m	30.69	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	188225	29.74	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	231485	31.25	ng/ul	0.00
52) 4-Nitrophenol-d4	14.53	143	25964m	25.53	ng/ul	0.00
58) Fluorene-d10	15.29	176	166941	31.02	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.43	200	16709	15.97	ng/ul	0.00
71) Anthracene-d10	17.14	188	268415	32.16	ng/ul	0.00
79) Pyrene-d10	19.45	212	315946	35.95	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.34	264	246503	34.73	ng/ul	0.00

Target Compounds						Qvalue
45) Dimethylphthalate	13.75	163	57927	8.78	ng/ul	99
77) Fluoranthene	19.11	202	13841	1.19	ng/ul	100
80) Pyrene	19.47	202	17136	1.44	ng/ul	99
84) Bis(2-ethylhexyl)phthalate	21.16	149	9247	1.20	ng/ul#	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022416\
Data File : BM004394.D
Acq On : 24 Feb 2016 20:34
Operator : SJ/UM
Sample : H1515-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0311-S19-0312

Manual Integrations
APPROVED

UMANGI
2/25/2016 2:43:47 PM

Quant Time: Feb 25 02:49:02 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 25 02:09:59 2016
Response via : Initial Calibration

