


Data Path : Z:\HPCHEM1\BNA M\DATA\BM022416\
 Data File : BM004375.D
 Acq On : 24 Feb 2016 08:58
 Operator : SJ/UM
 Sample : DFTPP55
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP55

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
 Title : SVOA CALIBRATION
 Last Update : Thu Feb 25 02:09:59 2016

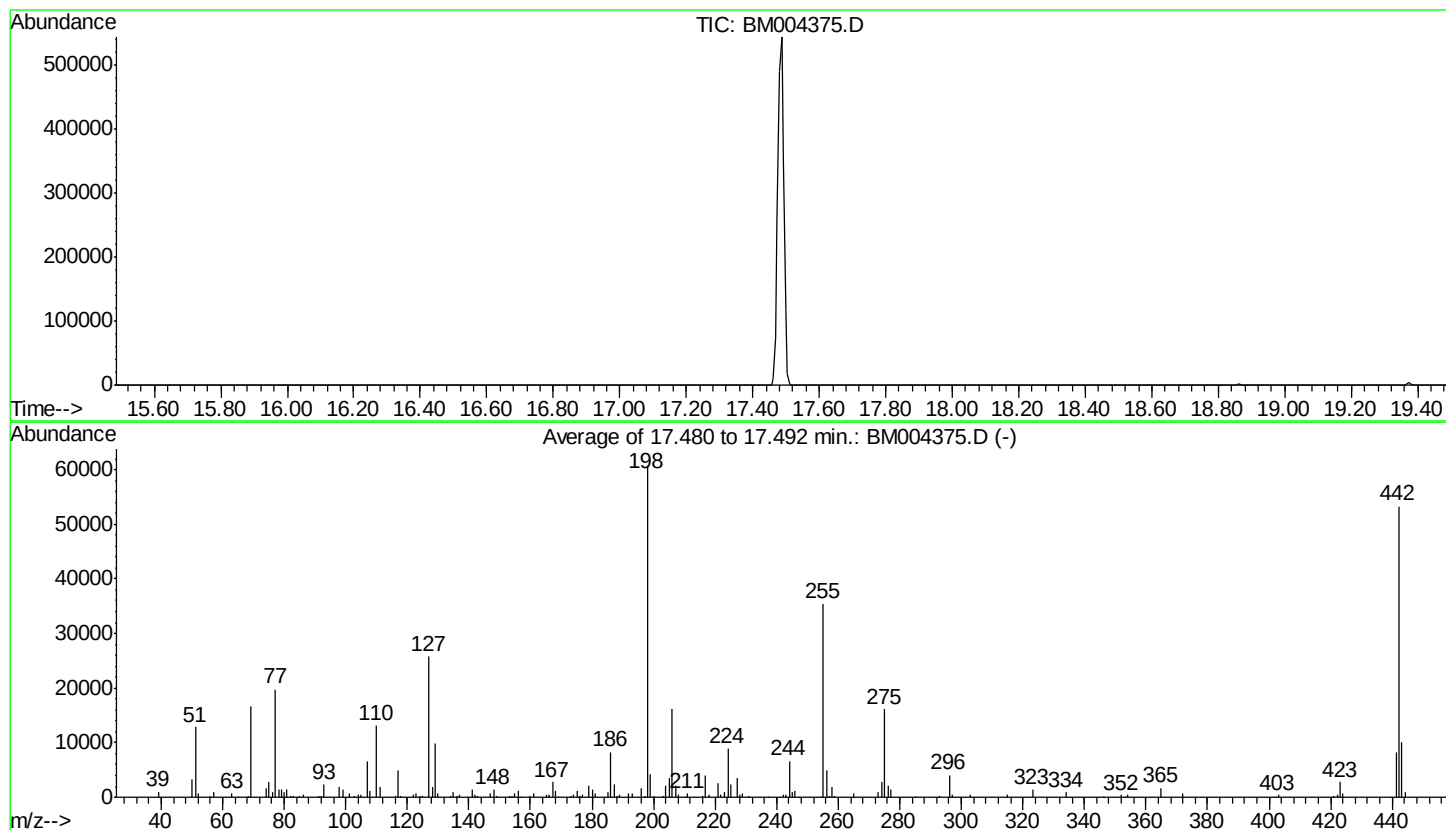

AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.2	12893	PASS
68	69	0.00	2	1.5	255	PASS
69	198	0.00	100	27.3	16580	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.5	25781	PASS
197	198	0.00	2	0.4	273	PASS
198	198	100	100	100.0	60730	PASS
199	198	5	9	6.8	4128	PASS
275	198	10	60	26.5	16094	PASS
365	198	1	100	2.8	1684	PASS
441	443	0.01	100	79.6	8106	PASS
442	198	50	100	87.7	53258	PASS
443	442	15	24	19.1	10187	PASS

m/z	Abundance
39.00	1218.0
50.10	3903.0
51.10	15489.0
52.10	713.0
56.00	485.0
57.00	1175.0
63.00	722.0
65.00	357.0
68.20	391.0
69.00	19408.0
74.10	1854.0
75.10	3288.0
76.10	1139.0
77.10	23312.0
78.10	1632.0
79.00	1633.0
80.00	1201.0
81.00	1674.0
82.00	393.0
83.00	382.0
85.00	432.0
86.00	473.0
91.00	392.0
92.10	428.0
93.00	2631.0
98.00	2041.0
99.00	1768.0
101.00	877.0
102.90	309.0
104.00	720.0
105.00	611.0
107.10	7550.0
108.00	1335.0
110.00	14939.0
111.10	2291.0
116.00	406.0
117.00	5819.0
118.00	415.0
122.00	536.0
123.00	831.0
124.00	323.0
124.90	355.0
127.10	28960.0
128.00	2219.0
129.00	10888.0
130.00	943.0
134.00	357.0
135.00	928.0
136.00	403.0
137.10	495.0
141.00	1479.0
142.00	513.0
142.90	308.0
147.00	776.0
148.00	1633.0
149.00	321.0
153.00	484.0
154.00	337.0
155.00	840.0
156.00	1316.0
160.00	468.0
161.00	699.0
165.00	503.0
166.00	504.0
167.10	3066.0
168.10	1481.0
169.00	309.0
173.10	370.0
174.00	620.0
175.10	1203.0
176.00	382.0
176.90	603.0
179.00	2297.0
180.10	1506.0
181.00	754.0
185.10	1055.0
186.10	8753.0
187.10	2668.0
188.10	300.0
189.00	499.0
192.00	709.0
193.00	783.0
196.00	1790.0
198.00	65232.0
199.00	4549.0
200.00	351.0
203.00	439.0
204.00	2230.0
205.10	3800.0
206.10	17080.0
207.10	2399.0
208.10	575.0

Instrument :
BNA_M
ClientSampleId :
DFTPP55

211.00	624.0
216.00	355.0
217.00	4230.0
218.00	543.0
221.10	2654.0
221.80	637.0
223.10	882.0
224.10	9217.0
225.10	2344.0
227.10	3607.0
228.00	536.0
229.00	751.0
231.00	340.0
242.10	432.0
243.10	492.0
244.10	6965.0
245.10	856.0
246.10	1320.0
255.10	36208.0
256.10	5064.0
257.00	447.0
258.10	1939.0
259.00	313.0
265.10	668.0
273.10	1010.0
274.10	2677.0
275.10	16294.0
276.10	2172.0
277.00	1405.0
293.00	320.0
296.10	4122.0
297.10	549.0
303.10	463.0
315.00	413.0
323.10	1332.0
334.10	796.0
352.10	379.0
354.10	378.0
365.00	1603.0
372.10	569.0
403.00	334.0
422.10	337.0
423.10	2443.0
424.10	638.0
441.20	6907.0
442.20	45056.0
443.20	8787.0
444.10	861.0

Instrument :
BNA_M
ClientSampleId :
DFTPP55

m/z	Abundance
39.10	1020.0
50.10	3748.0
51.10	14892.0
52.00	738.0
56.00	468.0
57.00	1127.0
63.00	768.0
68.20	374.0
69.00	19208.0
74.00	1916.0
75.10	3101.0
76.10	1015.0
77.10	22736.0
78.10	1598.0
79.00	1485.0
80.00	1141.0
81.00	1711.0
82.00	388.0
83.00	364.0
85.00	476.0
86.00	457.0
91.00	436.0
92.10	457.0
93.00	2640.0
98.00	2075.0
99.00	1703.0
101.00	954.0
103.00	326.0
104.00	627.0
105.00	638.0
107.10	7637.0
108.00	1190.0
110.00	15258.0
111.00	2182.0
116.10	457.0
117.10	5825.0
118.00	410.0
122.00	579.0
123.00	812.0
123.90	352.0
125.00	376.0
127.10	30000.0
128.10	2260.0
129.00	11561.0
130.00	912.0
134.00	366.0
135.00	1023.0
136.00	412.0
137.10	437.0
141.00	1636.0
142.00	466.0
143.00	318.0
147.00	831.0
148.00	1629.0
148.90	323.0
153.00	451.0
154.00	378.0
155.00	854.0
156.10	1322.0
157.10	308.0
160.00	486.0
161.10	733.0
165.10	589.0
166.00	428.0
167.10	3162.0
168.00	1401.0
173.10	353.0
174.00	672.0
175.10	1202.0
176.10	392.0
177.00	664.0
179.00	2427.0
180.00	1657.0
181.00	739.0
185.00	1198.0
186.10	9668.0
187.10	2610.0
188.10	361.0
189.00	555.0
192.00	722.0
193.10	905.0
196.10	1973.0
197.10	452.0
198.00	70352.0
199.00	4829.0
200.00	387.0
203.00	457.0
204.10	2389.0
205.10	4006.0
206.10	18888.0
207.10	2556.0
208.00	614.0

Instrument :
BNA_M
ClientSampleId :
DFTPP55

210.20	368.0
211.00	726.0
216.00	387.0
217.00	4647.0
218.00	567.0
221.10	3045.0
221.80	680.0
223.10	977.0
224.10	10382.0
225.10	2676.0
227.10	4166.0
228.10	543.0
229.00	820.0
231.10	356.0
237.00	365.0
242.00	505.0
243.10	591.0
244.10	7781.0
245.10	1062.0
246.00	1583.0
247.00	342.0
255.10	41352.0
256.10	5807.0
257.00	473.0
258.10	2127.0
259.00	339.0
265.10	940.0
273.10	1167.0
274.10	3342.0
275.10	18672.0
276.10	2369.0
277.10	1535.0
285.00	343.0
293.00	347.0
296.10	4689.0
297.00	697.0
303.10	580.0
315.00	517.0
323.10	1645.0
334.10	1049.0
346.10	351.0
352.10	466.0
353.10	301.0
354.00	518.0
365.10	1932.0
372.10	727.0
402.10	326.0
403.10	529.0
421.10	446.0
422.10	419.0
423.10	3207.0
424.10	768.0
441.20	9556.0
442.20	62736.0
443.20	12147.0
444.10	1099.0

Instrument :
BNA_M
ClientSampleId :
DFTPP55

m/z	Abundance
39.10	598.0
50.10	1977.0
51.10	8299.0
52.00	457.0
57.00	583.0
63.00	446.0
69.00	11124.0
74.10	973.0
75.00	1799.0
76.10	594.0
77.10	13200.0
78.10	939.0
79.00	889.0
80.00	614.0
81.00	963.0
86.00	310.0
93.00	1600.0
98.00	1276.0
99.00	957.0
101.00	581.0
104.00	405.0
105.00	337.0
107.00	4716.0
108.00	718.0
110.00	9176.0
111.00	1422.0
117.00	3464.0
122.00	327.0
123.00	487.0
127.10	18384.0
128.00	1321.0
129.00	7123.0
130.00	564.0
135.00	567.0
137.00	302.0
141.00	919.0
142.10	333.0
147.00	497.0
148.00	957.0
155.00	589.0
156.00	863.0
161.00	464.0
165.00	391.0
166.00	330.0
167.10	1973.0
168.00	939.0
174.10	412.0
175.00	884.0
177.00	463.0
179.00	1505.0
180.10	1041.0
181.00	525.0
185.00	779.0
186.10	6265.0
187.10	1797.0
189.00	385.0
192.00	513.0
193.10	560.0
196.00	1179.0
197.10	369.0
198.00	46608.0
199.00	3006.0
200.00	301.0
204.10	1582.0
205.10	2809.0
206.10	12571.0
207.10	1647.0
208.00	416.0
211.10	506.0
217.00	3172.0
218.00	383.0
221.00	1943.0
221.80	453.0
223.00	696.0
224.10	6846.0
225.10	1784.0
227.10	2750.0
228.00	374.0
229.00	575.0
242.10	366.0
243.10	373.0
244.10	5304.0
245.10	709.0
246.00	962.0
254.20	301.0
255.10	28832.0
256.10	3841.0
258.00	1630.0
265.00	593.0
273.00	779.0
274.10	2369.0
275.10	13318.0

Instrument :
BNA_M
ClientSampleId :
DFTPP55

276.10	1680.0
277.10	1092.0
296.10	3413.0
297.10	402.0
303.00	434.0
315.10	362.0
323.10	1196.0
334.10	740.0
352.00	327.0
354.10	380.0
365.10	1519.0
372.10	663.0
403.10	392.0
421.10	328.0
422.10	329.0
423.10	2468.0
424.10	573.0
441.20	7855.0
442.20	51984.0
443.10	9628.0
444.10	905.0

Instrument :
BNA_M
ClientSampleId :
DFTPP55