

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022417\
 Data File : BM009011.D
 Acq On : 24 Feb 2017 11:00
 Operator : SJ/MA
 Sample : PB97145BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK45

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022317.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	43	47	51	rBV	84909	93658	1.87%	0.177%
2	7.057	667	675	685	rBV	1126385	1770236	35.39%	3.337%
3	7.234	697	705	714	rBV	827361	1296423	25.92%	2.444%
4	7.434	732	739	750	rVB	1091093	1720870	34.40%	3.244%
5	7.904	812	819	829	rBV	745019	1168795	23.36%	2.203%
6	8.598	928	937	947	rBV	1261152	2011331	40.21%	3.792%
7	9.069	1009	1017	1026	rBV	1056311	1739793	34.78%	3.280%
8	9.786	1133	1139	1152	rVB	845417	1422455	28.43%	2.681%
9	10.316	1222	1229	1242	rBV	1197647	2025584	40.49%	3.818%
10	10.704	1288	1295	1303	rBV	892604	1495414	29.89%	2.819%
11	10.845	1311	1319	1329	rBV	1150920	1991093	39.80%	3.753%
12	13.945	1840	1846	1856	rVB	2064948	2823290	56.44%	5.322%
13	14.239	1889	1896	1904	rBV	2197777	3181544	63.60%	5.997%
14	14.545	1940	1948	1955	rVB2	1250949	1884887	37.68%	3.553%
15	14.727	1973	1979	1990	rBV	1099438	1511699	30.22%	2.850%
16	15.533	2110	2116	2127	rBV	2833235	4008317	80.13%	7.556%
17	15.645	2129	2135	2148	rVB	883998	1283000	25.65%	2.419%
18	17.286	2407	2414	2421	rBV	1592647	2254728	45.07%	4.250%
19	17.386	2424	2431	2440	rBV	3137839	4379097	87.54%	8.255%
20	19.309	2752	2758	2765	rBV5	31803	57948	1.16%	0.109%
21	19.674	2814	2820	2829	rBV	3829631	5002489	100.00%	9.430%
22	21.456	3118	3123	3128	rBV	2227323	2692060	53.81%	5.075%
23	23.656	3490	3497	3508	rVB2	2461559	4706560	94.08%	8.872%
24	23.803	3516	3522	3532	rVB2	1301222	2526659	50.51%	4.763%


Sum of corrected areas: 53047930

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022417\
Data File : BM009011.D
Acq On : 24 Feb 2017 11:00
Operator : SJ/MA
Sample : PB97145BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK45

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM022317.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

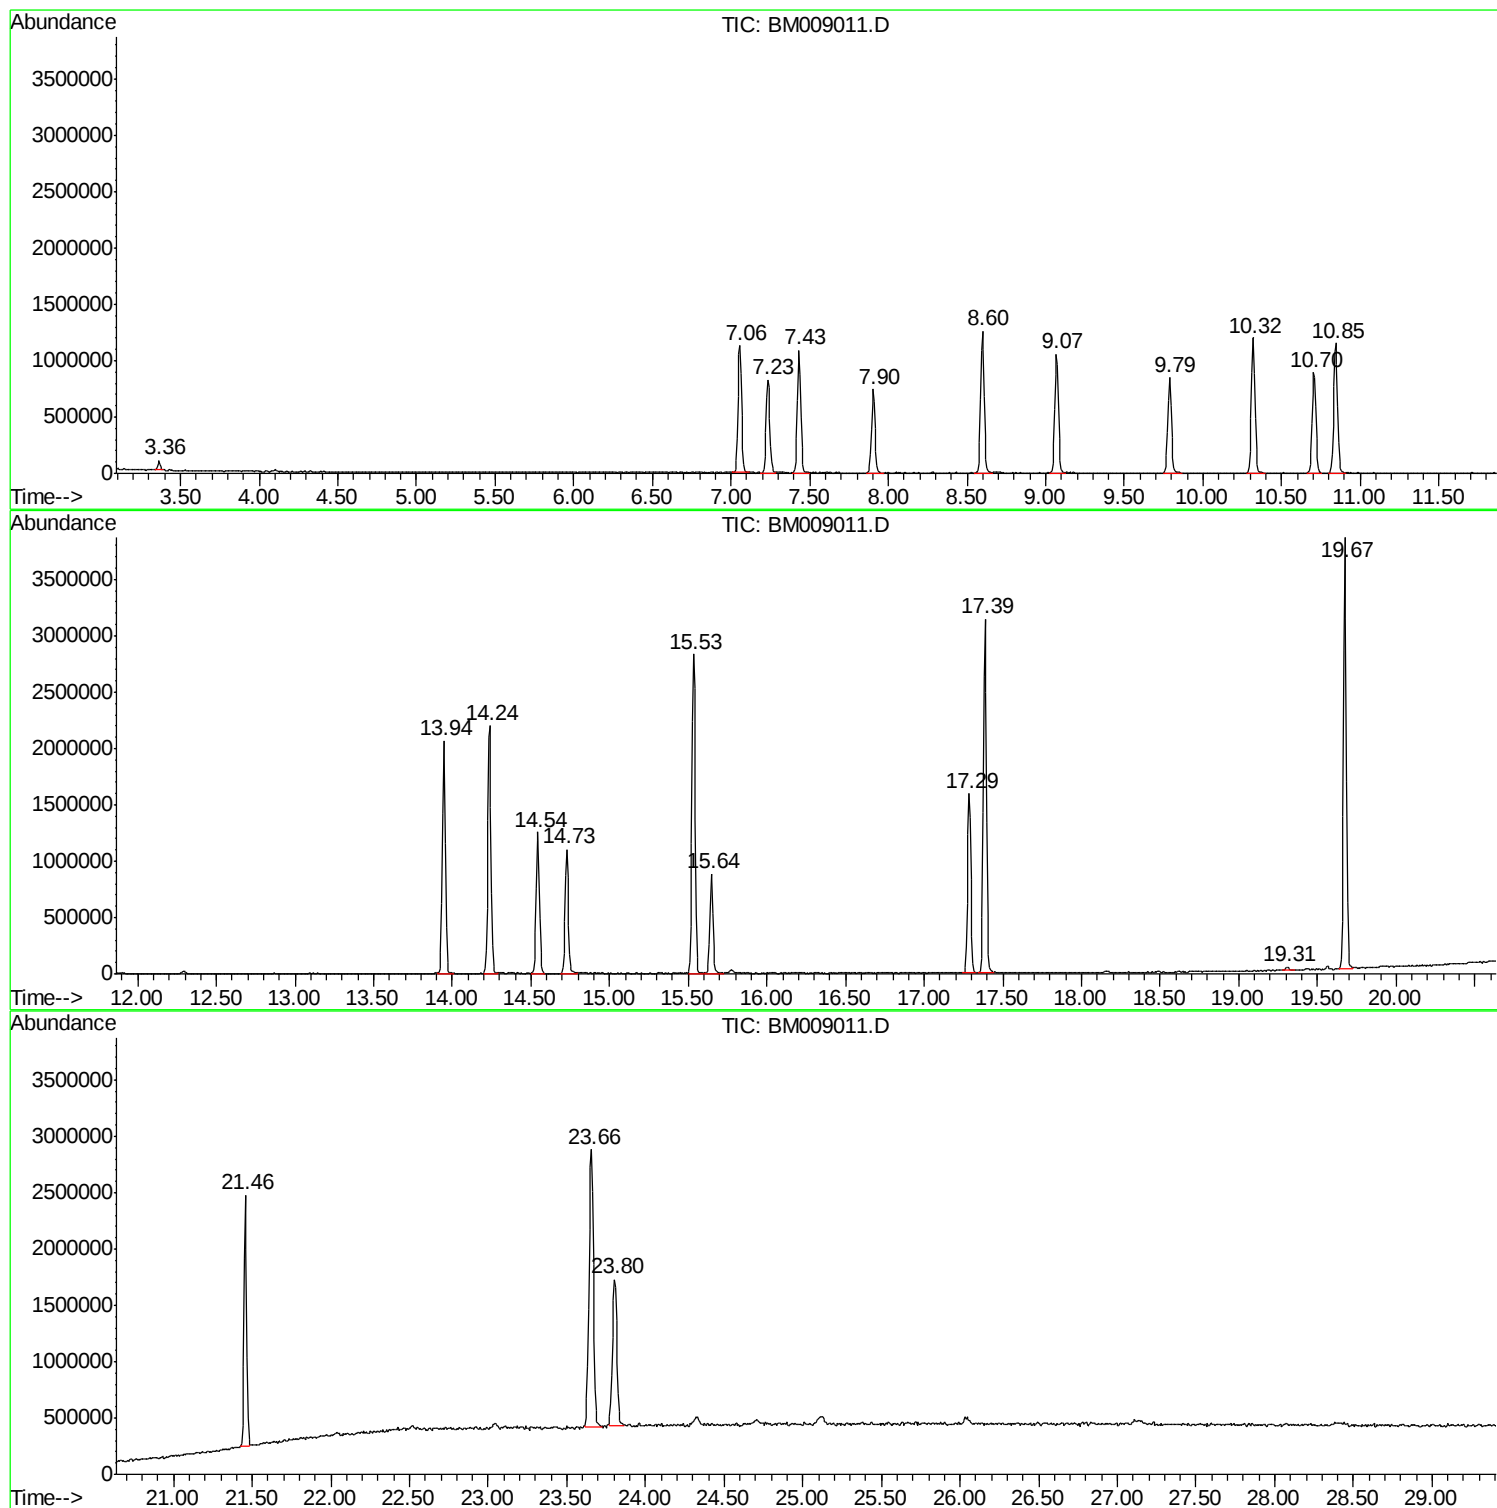

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022417\
Data File : BM009011.D
Acq On : 24 Feb 2017 11:00
Operator : SJ/MA
Sample : PB97145BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK45

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022317.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022417\
Data File : BM009011.D
Acq On : 24 Feb 2017 11:00
Operator : SJ/MA
Sample : PB97145BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK45

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022317.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc