

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022417\
 Data File : BM009013.D
 Acq On : 24 Feb 2017 12:13
 Operator : SJ/MA
 Sample : I1940-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DABP6

Quant Time: Feb 24 13:19:46 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022317.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 24 13:06:22 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	172766	20.00	ng/ul	0.00
18) Naphthalene-d8	10.70	136	645946	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.54	164	392277	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.29	188	933289	20.00	ng/ul	0.00
75) Chrysene-d12	21.45	240	1147967	20.00	ng/ul	0.00
83) Perylene-d12	23.80	264	1084646	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.36	96	20891	4.86	ng/uL	0.00
5) Phenol-d5	7.05	99	390468	24.94	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.23	67	301550	26.89	ng/ul	0.00
9) 2-Chlorophenol-d4	7.43	132	266612	25.55	ng/ul	0.00
13) 4-Methylphenol-d8	8.59	113	294645	25.63	ng/ul	0.00
19) Nitrobenzene-d5	9.06	128	129882	28.10	ng/ul	0.00
22) 2-Nitrophenol-d4	9.78	143	140568	28.18	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.32	165	275422	26.30	ng/ul	0.00
29) 4-Chloroaniline-d4	10.84	131	336449	30.48	ng/ul	0.00
43) Dimethylphthalate-d6	13.95	166	856310	32.42	ng/ul	0.00
46) Acenaphthylene-d8	14.23	160	1022244	31.51	ng/ul	0.00
51) 4-Nitrophenol-d4	14.72	143	120091	26.04	ng/ul	0.00
57) Fluorene-d10	15.53	176	768214	31.15	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.65	200	120206	21.40	ng/ul	0.00
70) Anthracene-d10	17.38	188	1247258	28.23	ng/ul	0.00
76) Pyrene-d10	19.67	212	1468461	29.34	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.65	264	1423621	28.91	ng/ul	0.00


Target Compounds						Qvalue
6) Phenol	7.08	94	65682	3.97	ng/ul#	74
44) Dimethylphthalate	13.99	163	210683	7.97	ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022417\
Data File : BM009013.D
Acq On : 24 Feb 2017 12:13
Operator : SJ/MA
Sample : I1940-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DABP6

Quant Time: Feb 24 13:19:46 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022317.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 24 13:06:22 2017
Response via : Initial Calibration

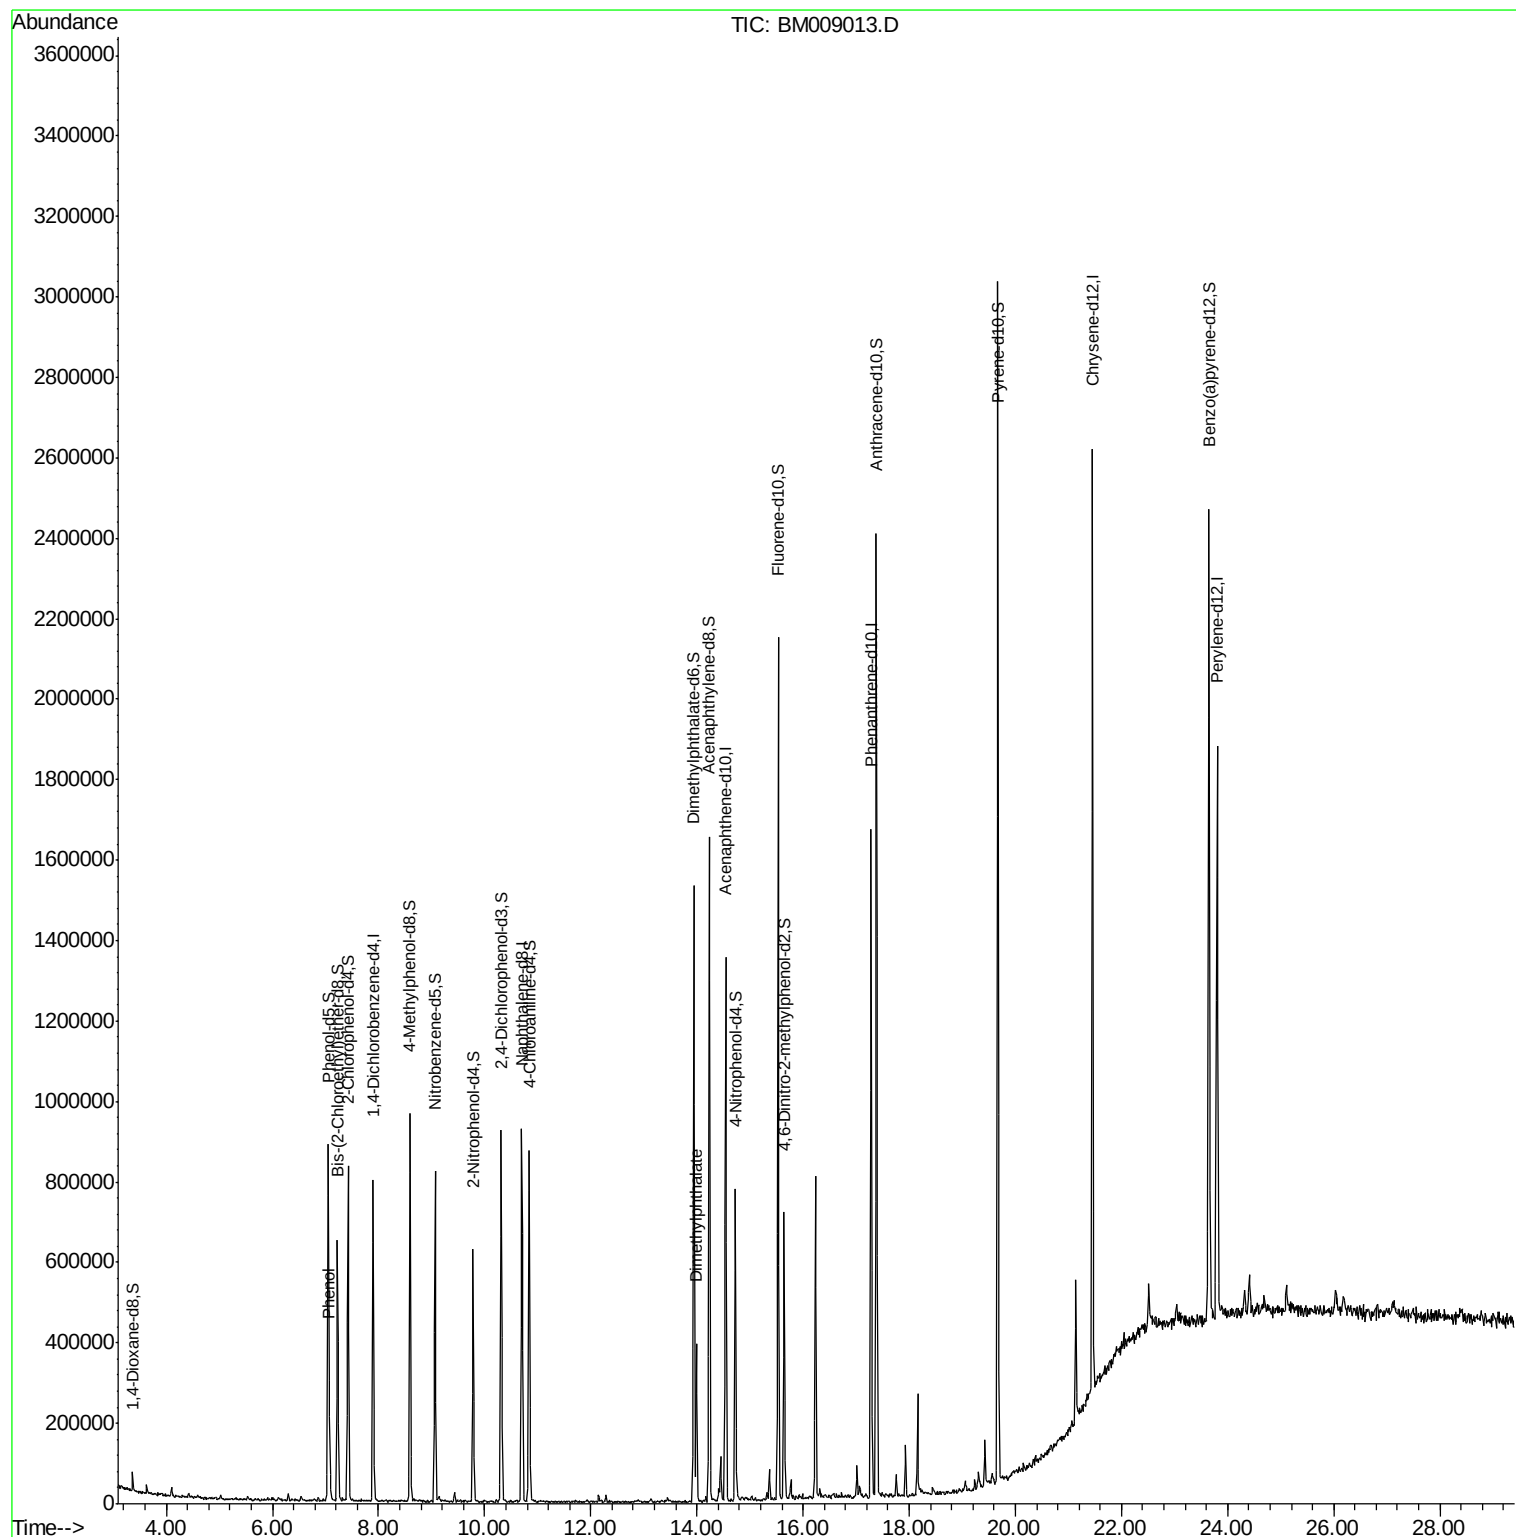

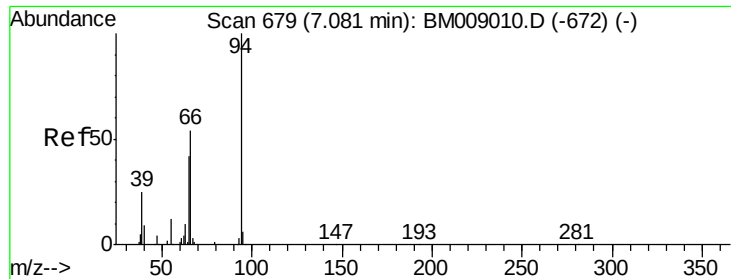

#6

Phenol

Concen: 3.97 ng/ul

RT: 7.08 min Scan# 678

Delta R.T. -0.01 min

Lab File: BM009013.D

Acq: 24 Feb 2017 12:13

Instrument :

BNA_M

ClientSampled :

DABP6


Tgt Ion: 94 Resp: 65682

Ion Ratio Lower Upper

94 100

65 39.1 39.8 59.6#

66 58.2 69.9 104.9#

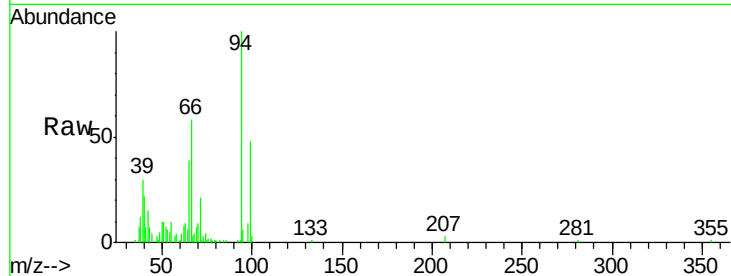

Abundance Ion 94.00 (93.70 to 94.70): BM009010.D (-672) (-)

Ion 65.00 (64.70 to 65.70): BM009010.D (-672) (-)

Ion 66.00 (65.70 to 66.70): BM009010.D (-672) (-)

Time-->

7.08

7.05

7.10

7.15

7.20

7.25

7.30

7.35

7.40

7.45

7.50

7.55

7.60

7.65

7.70

7.75

7.80

7.85

7.90

7.95

8.00

8.05

8.10

8.15

8.20

8.25

8.30

8.35

8.40

8.45

8.50

8.55

8.60

8.65

8.70

8.75

8.80

8.85

8.90

8.95

9.00

9.05

9.10

9.15

9.20

9.25

9.30

9.35

9.40

9.45

9.50

9.55

9.60

9.65

9.70

9.75

9.80

9.85

9.90

9.95

10.00

10.05

10.10

10.15

10.20

10.25

10.30

10.35

10.40

10.45

10.50

10.55

10.60

10.65

10.70

10.75

10.80

10.85

10.90

10.95

11.00

11.05

11.10

11.15

11.20

11.25

11.30

11.35

11.40

11.45

11.50

11.55

11.60

11.65

11.70

11.75

11.80

11.85

11.90

11.95

12.00

12.05

12.10

12.15

12.20

12.25

12.30

12.35

12.40

12.45

12.50

12.55

12.60

12.65

12.70

12.75

12.80

12.85

12.90

12.95

13.00

13.05

13.10

13.15

13.20

13.25

13.30

13.35

13.40

13.45

13.50

13.55

13.60

13.65

13.70

13.75

13.80

13.85

13.90

13.95

14.00

14.05

14.10

14.15

14.20

14.25

14.30

14.35

14.40

14.45

14.50

14.55

14.60

14.65

14.70

14.75

14.80

14.85

14.90

14.95

15.00

15.05

15.10

15.15

15.20

15.25

15.30

15.35

15.40

15.45

15.50

15.55

15.60

15.65

15.70

15.75

15.80

15.85

15.90

15.95

16.00

16.05

16.10

16.15

16.20

16.25

16.30

16.35

16.40

16.45

16.50

16.55

16.60

16.65

16.70

16.75

16.80

16.85

16.90

16.95

17.00

17.05

17.10

17.15

17.20

17.25

17.30

17.35

17.40

17.45

17.50

17.55

17.60

17.65

17.70

17.75

17.80

17.85

17.90

17.95

18.00

18.05

18.10

18.15

18.20

18.25

18.30

18.35

18.40

18.45

18.50

18.55

18.60

18.65

18.70

18.75

18.80

18.85

18.90

18.95

19.00

19.05

19.10

19.15

19.20

19.25

19.30

19.35

19.40

19.45

19.50

19.55

19.60

19.65

19.70

19.75

19.80

19.85