

Data Path : Z:\HPCHEM1\BNA_M\Data\BM022417\
 Data File : BM009023.D
 Acq On : 24 Feb 2017 19:02
 Operator : SJ/MA
 Sample : I1943-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DABQ1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022317.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	35	41	50	rBV	1029845	1523591	3.03%	1.620%
2	4.622	250	261	276	rBV	35966725	50308766	100.00%	53.492%
3	7.228	698	704	712	rBV	625339	969020	1.93%	1.030%
4	7.428	730	738	746	rBV	690577	1090375	2.17%	1.159%
5	7.898	811	818	824	rBV	679163	1094275	2.18%	1.164%
6	8.592	930	936	947	rVB	514498	796282	1.58%	0.847%
7	9.063	1006	1016	1026	rBV	800993	1355983	2.70%	1.442%
8	9.781	1129	1138	1147	rBV	665906	1103999	2.19%	1.174%
9	10.316	1221	1229	1238	rBV	929013	1529383	3.04%	1.626%
10	10.704	1287	1295	1301	rBV	820330	1406209	2.80%	1.495%
11	13.945	1839	1846	1851	rBV	1713801	2343718	4.66%	2.492%
12	14.233	1888	1895	1903	rBV	1742207	2466535	4.90%	2.623%
13	14.539	1941	1947	1954	rBV3	1140759	1731801	3.44%	1.841%
14	15.533	2109	2116	2122	rBV	2258557	3301664	6.56%	3.511%
15	15.645	2129	2135	2144	rBV	912545	1238045	2.46%	1.316%
16	17.286	2407	2414	2424	rBV	1571916	2184234	4.34%	2.322%
17	17.386	2424	2431	2444	rVB	2622593	3799687	7.55%	4.040%
18	19.674	2814	2820	2832	rBV2	3538621	4741655	9.43%	5.042%
19	21.456	3118	3123	3129	rBV	2410760	2957135	5.88%	3.144%
20	23.650	3489	3496	3508	rVB2	2676287	5153964	10.24%	5.480%
21	23.803	3515	3522	3529	rBV	1540479	2952521	5.87%	3.139%




Sum of corrected areas: 94048842

Data Path : Z:\HPCHEM1\BNA_M\Data\BM022417\
Data File : BM009023.D
Acq On : 24 Feb 2017 19:02
Operator : SJ/MA
Sample : I1943-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DABQ1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022317.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

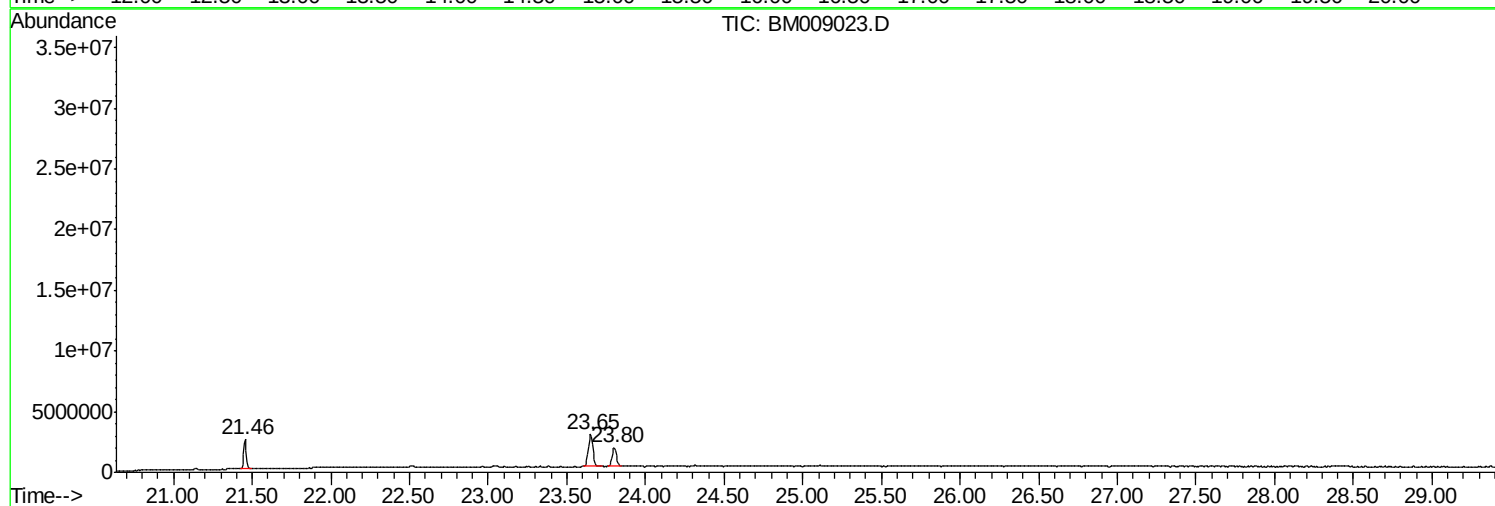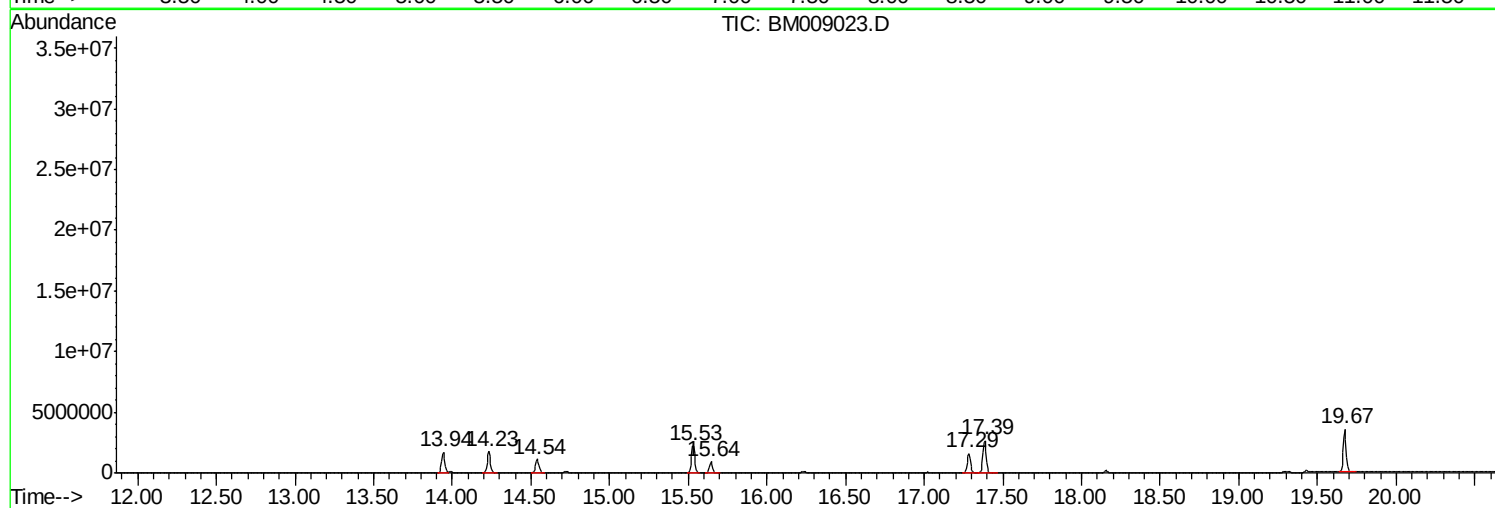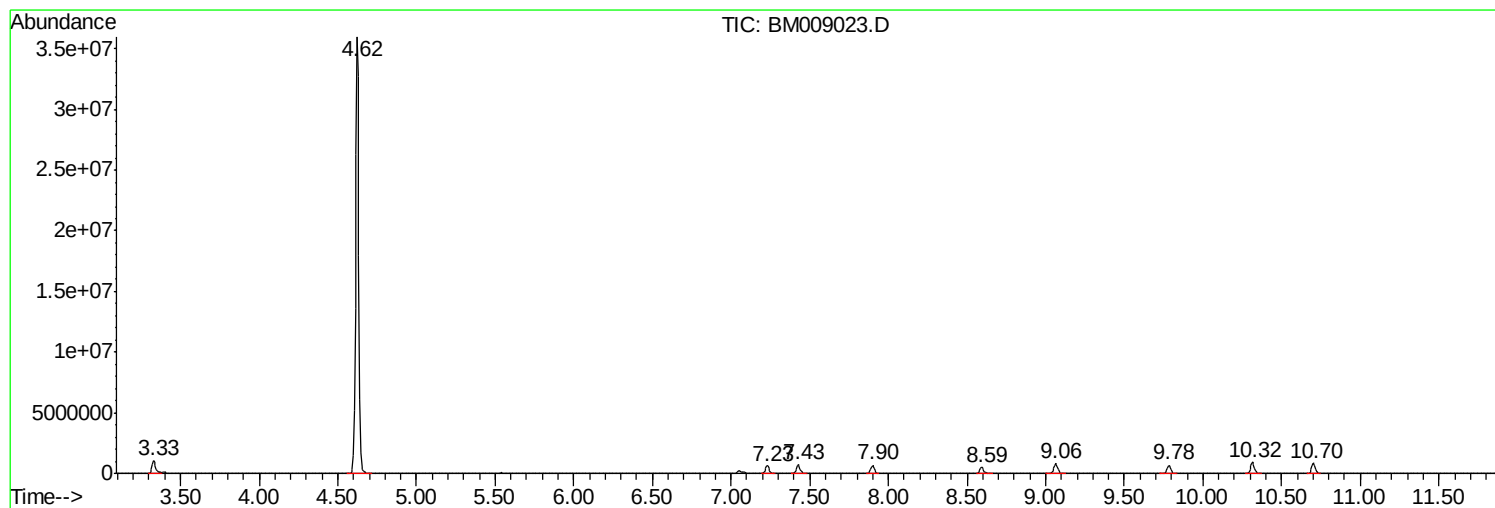

Data Path : Z:\HPCHEM1\BNA_M\Data\BM022417\
Data File : BM009023.D
Acq On : 24 Feb 2017 19:02
Operator : SJ/MA
Sample : I1943-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DABQ1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022317.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\Data\BM022417\
Data File : BM009023.D
Acq On : 24 Feb 2017 19:02
Operator : SJ/MA
Sample : I1943-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DABQ1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022317.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc