

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022421\
 Data File : BM028878.D
 Acq On : 24 Feb 2021 13:42
 Operator : CG/JU
 Sample : PB134792BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB134792BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM028878.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.363	398	404	415	rBV	402679	560445	49.78%	10.971%
2	6.998	675	682	696	rBV	370704	571997	50.81%	11.197%
3	7.804	814	819	827	rBB	68056	102677	9.12%	2.010%
4	8.987	1013	1020	1031	rBB	226175	356771	31.69%	6.984%
5	10.610	1289	1296	1305	rBB	88554	141611	12.58%	2.772%
6	13.086	1710	1717	1723	rBV	557143	788205	70.01%	15.430%
7	14.469	1946	1952	1958	rBB	131479	184762	16.41%	3.617%
8	15.963	2200	2206	2214	rBB	464644	609865	54.17%	11.939%
9	17.210	2412	2418	2425	rBV	162521	215005	19.10%	4.209%
10	19.827	2857	2863	2868	rBV	937429	1125848	100.00%	22.040%
11	21.368	3120	3125	3132	rBV	195735	233616	20.75%	4.573%
12	23.580	3495	3501	3508	rBV2	119433	217494	19.32%	4.258%




Sum of corrected areas: 5108296

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022421\
Data File : BM028878.D
Acq On : 24 Feb 2021 13:42
Operator : CG/JU
Sample : PB134792BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB134792BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

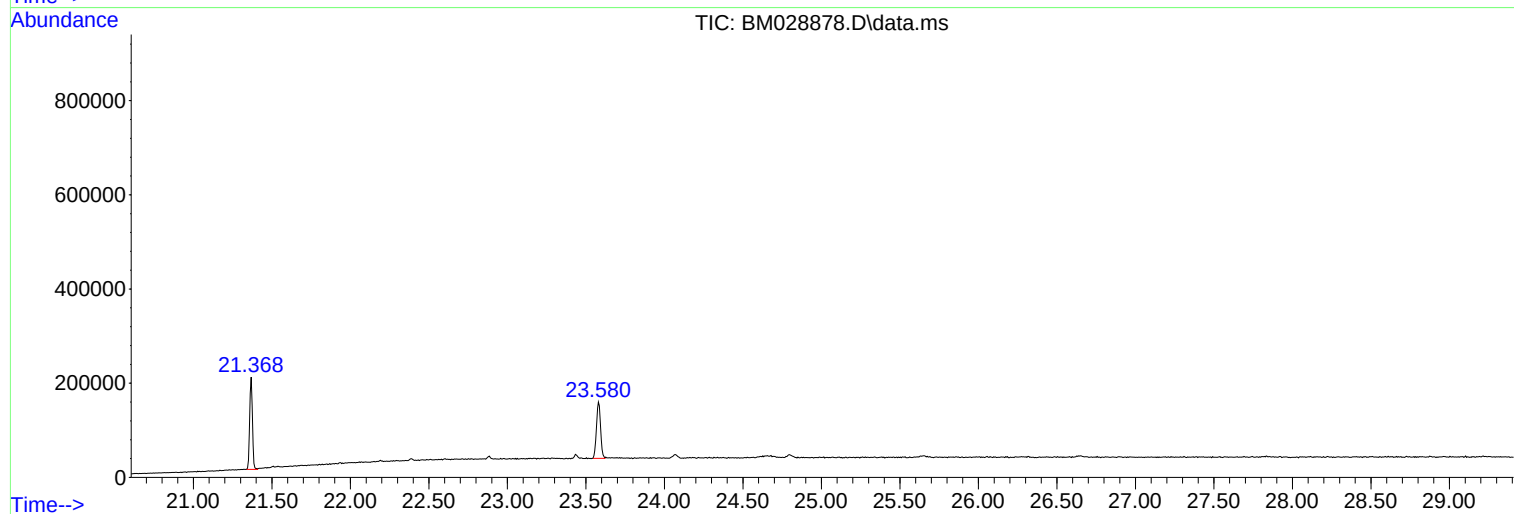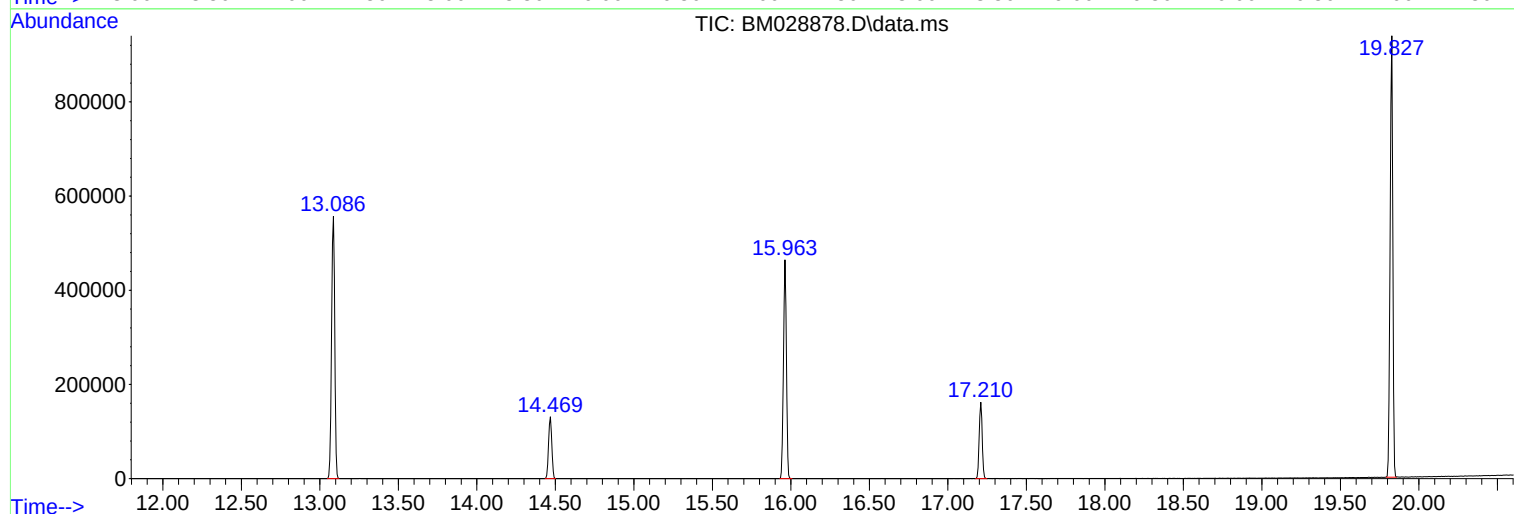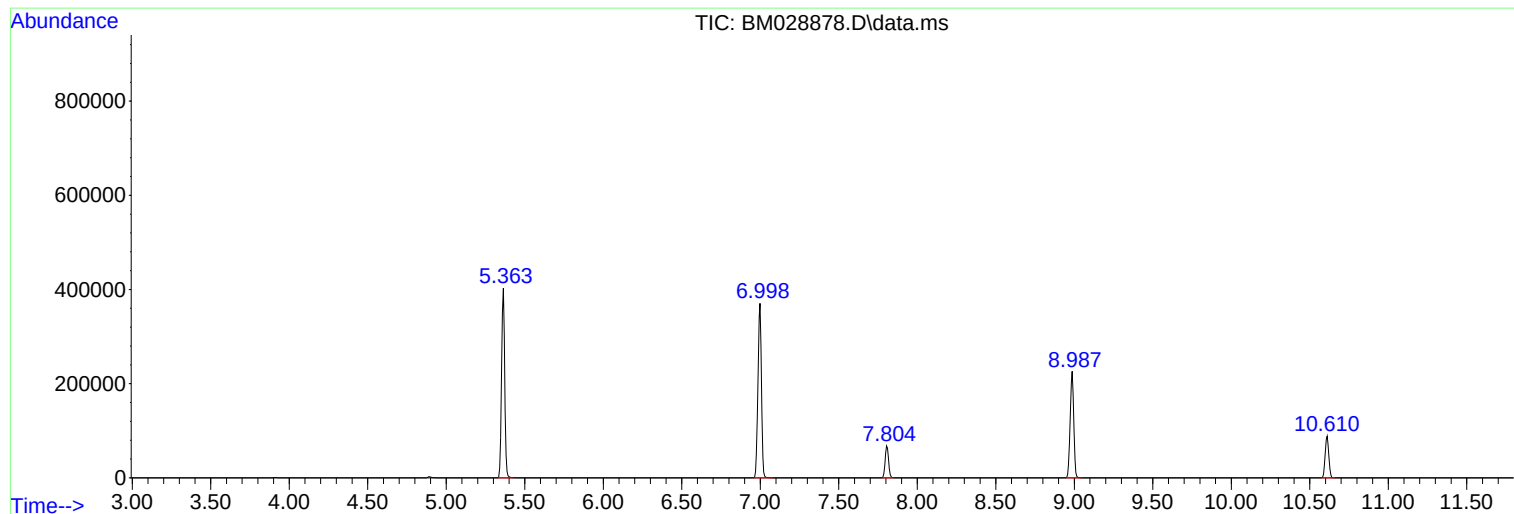

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022421\
Data File : BM028878.D
Acq On : 24 Feb 2021 13:42
Operator : CG/JU
Sample : PB134792BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB134792BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022421\
Data File : BM028878.D
Acq On : 24 Feb 2021 13:42
Operator : CG/JU
Sample : PB134792BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB134792BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------