


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022421\
 Data File : BM028876.D
 Acq On : 24 Feb 2021 12:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 23 16:39:41 2021

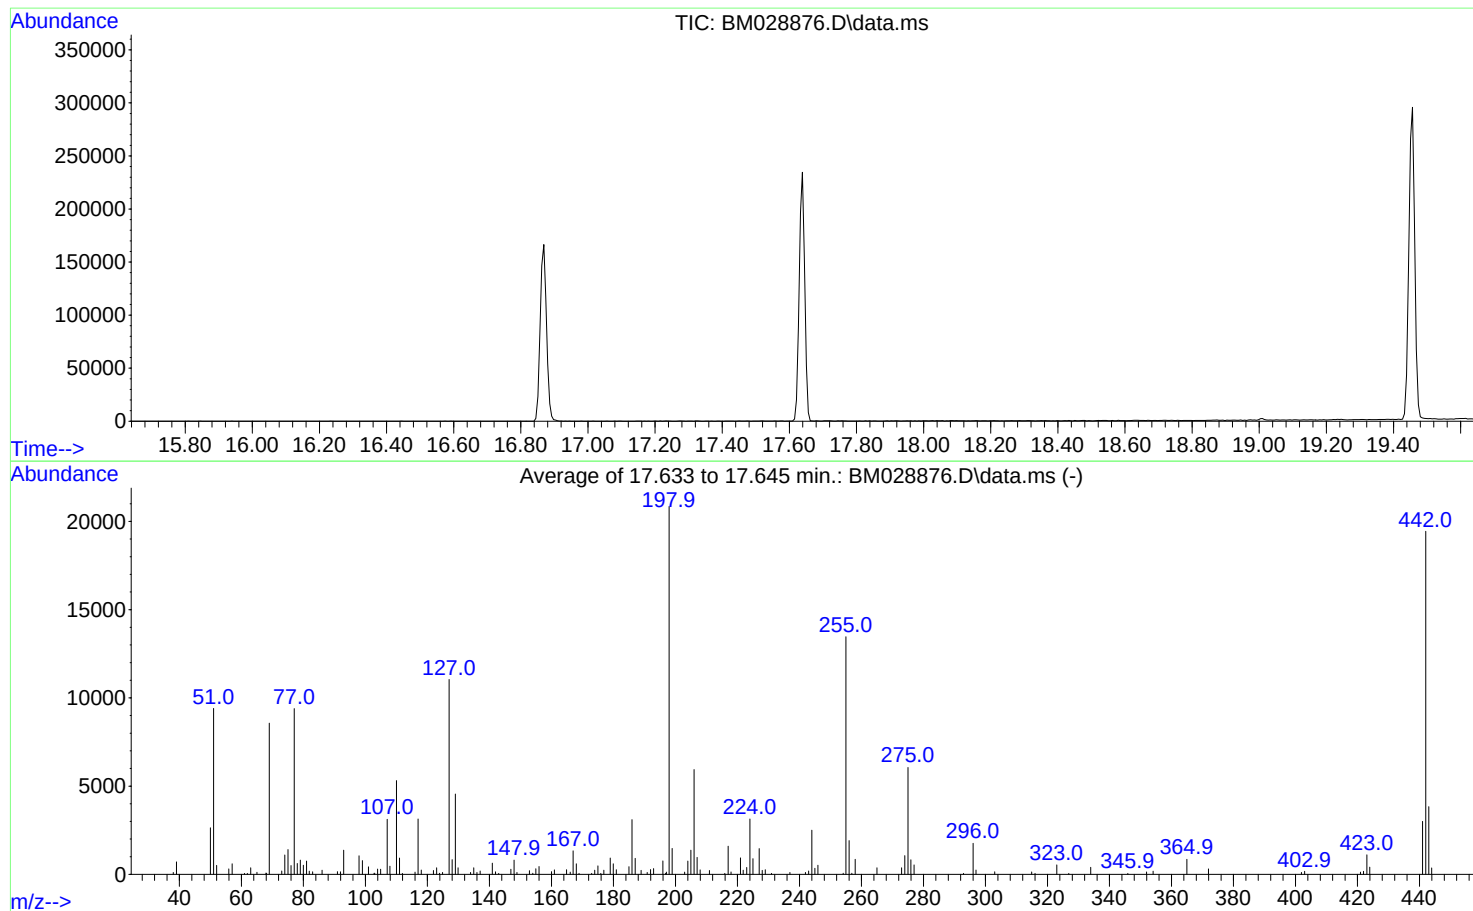

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.1	9400	PASS
68	69	0.00	2	0.8	71	PASS
69	198	0.00	100	41.1	8565	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.0	11046	PASS
197	198	0.00	2	0.6	127	PASS
198	198	100	100	100.0	20845	PASS
199	198	5	9	7.0	1468	PASS
275	198	10	60	29.1	6060	PASS
365	198	1	100	4.1	853	PASS
441	198	0.01	100	14.4	3004	PASS
442	442	50	100	100.0	19437	PASS
443	442	15	24	19.8	3839	PASS




Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

	DDT Breakdown	
Date	Instrument Name	DFTPP Data File
2/24/2021	BNA_M	<u>BM028876.D</u>
Compound Name	Response	Retention Time
DDT	72913	20.668
DDD	241	20.274
DDE	0	19.821
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
241	73154	0.33

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022421\
Data File : BM028876.D
Acq On : 24 Feb 2021 12:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 24 13:23:45 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 23 16:39:41 2021
Response via : Initial Calibration

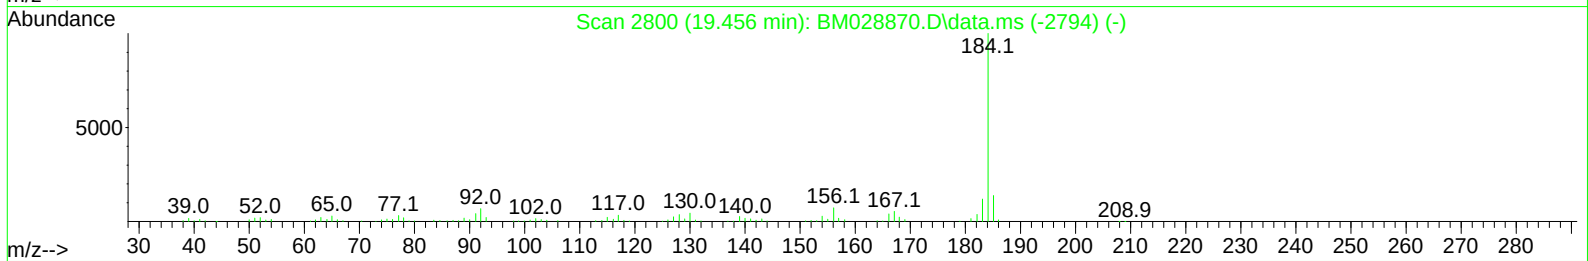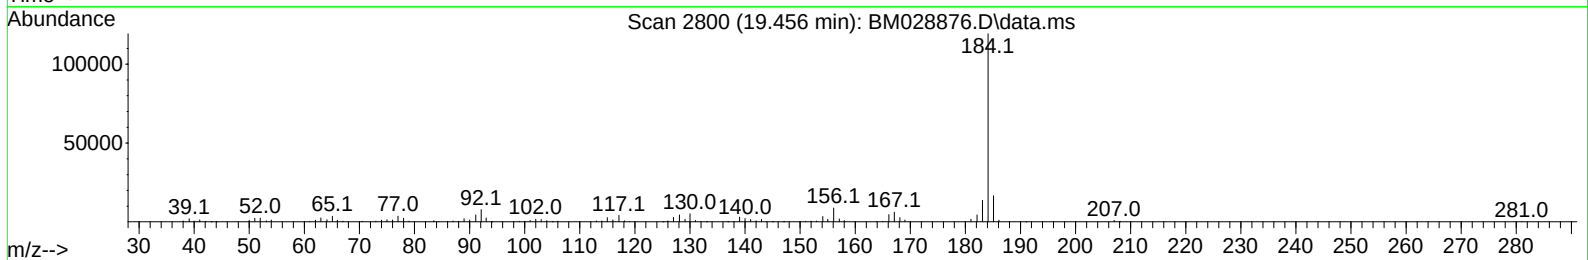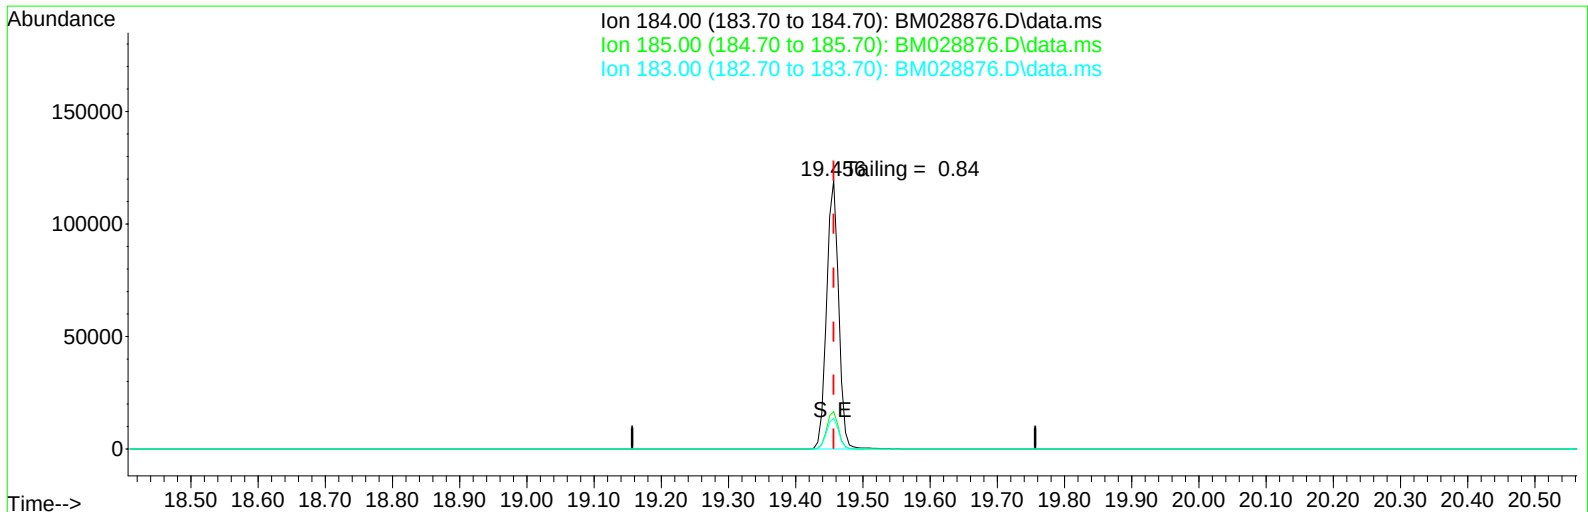

TIC: BM028876.D\data.ms

(77) Benzidine

19.456min (-0.000) 0.00 ng




response 147914

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	13.98
183.00	12.10	11.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022421\
Data File : BM028876.D
Acq On : 24 Feb 2021 12:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 24 13:23:45 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 23 16:39:41 2021
Response via : Initial Calibration

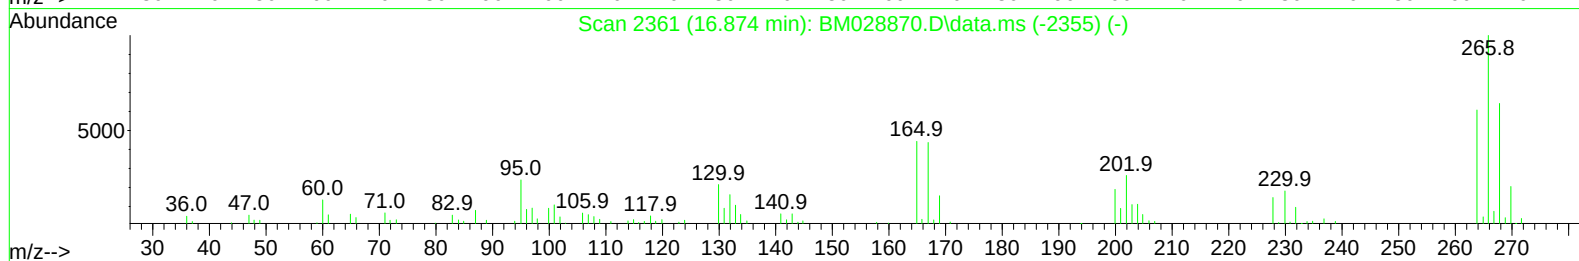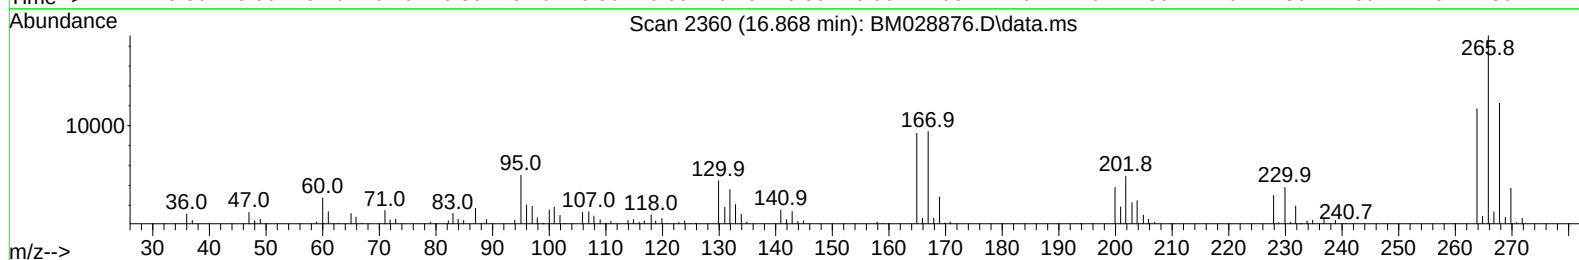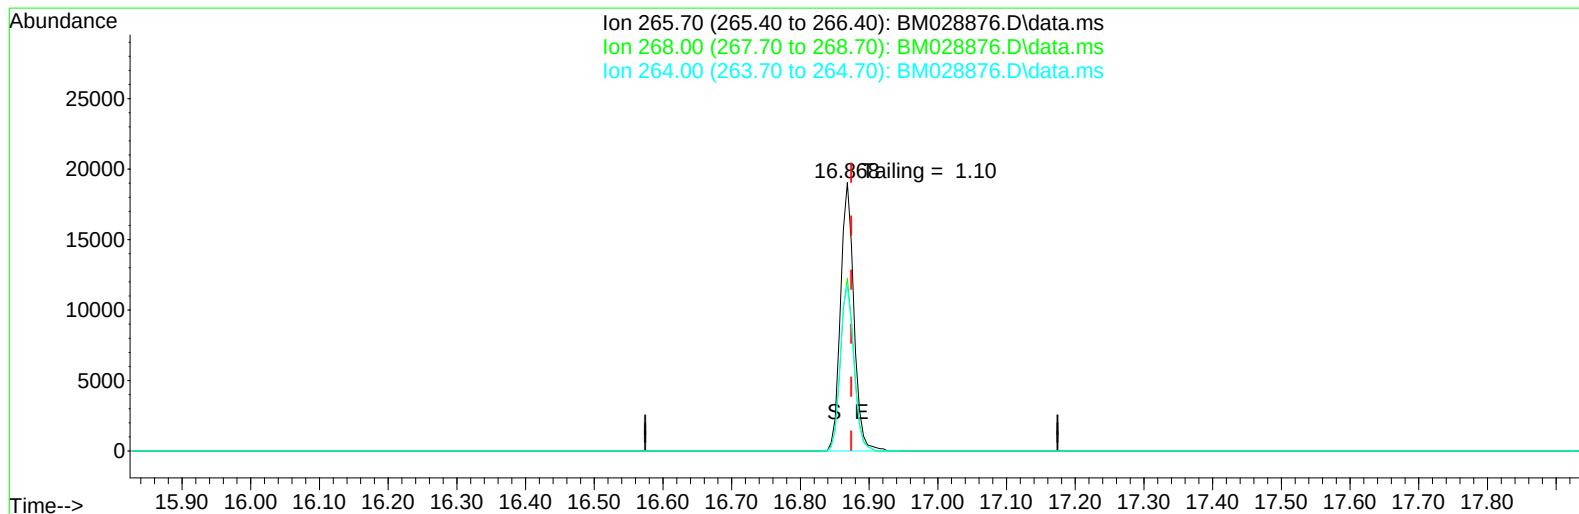

TIC: BM028876.D\data.ms

(70) Pentachlorophenol (C)

16.868min (-0.006) 0.00 ng

response 25704

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	64.35
264.00	63.30	61.53
0.00	0.00	0.00