

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
 Data File : BM044296.D
 Acq On : 24 Feb 2024 15:40
 Operator : MA/JU
 Sample : P1494-21
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3Z7

Quant Time: Feb 25 23:00:36 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Feb 25 22:57:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.916	152	278756	20.000	ng/ul	0.00
20) Naphthalene-d8	10.722	136	1222804	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.563	164	725584	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.315	188	1529412	20.000	ng/ul	0.00
79) Chrysene-d12	21.515	240	1353911	20.000	ng/ul	0.00
88) Perylene-d12	23.921	264	1451155	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	34006	3.849	ng/uL	0.00
4) Pyridine-d5	3.769	84	327014	13.553	ng/ul	0.00
7) Phenol-d5	7.081	99	197565	7.398	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.257	67	618465	35.765	ng/ul	0.00
11) 2-Chlorophenol-d4	7.446	132	551735	27.433	ng/ul	0.00
15) 4-Methylphenol-d8	8.634	113	58452	2.893	ng/ul	0.00
21) Nitrobenzene-d5	9.087	128	383119	38.534	ng/ul	0.00
24) 2-Nitrophenol-d4	9.810	143	400460	39.479	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.339	165	536545	29.986	ng/ul	0.00
31) 4-Chloroaniline-d4	10.875	131	224758	7.479	ng/ul	0.01
46) Dimethylphthalate-d6	13.986	166	2303103	41.156	ng/ul	0.00
49) Acenaphthylene-d8	14.257	160	2549617	39.600	ng/ul	0.00
54) 4-Nitrophenol-d4	14.769	143	81210	7.293	ng/ul	0.00
60) Fluorene-d10	15.557	176	1990462	42.024	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.680	200	345283	36.385	ng/ul	0.00
73) Anthracene-d10	17.415	188	2522270	34.587	ng/ul	0.00
81) Pyrene-d10	19.715	212	3679377	45.172	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.768	264	2794107	37.576	ng/ul	0.00


Target Compounds					Qvalue
86) Bis(2-ethylhexyl)phtha...	21.445	149	102369	1.453 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044296.D
Acq On : 24 Feb 2024 15:40
Operator : MA/JU
Sample : P1494-21
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3Z7

Quant Time: Feb 25 23:00:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Feb 25 22:57:38 2024
Response via : Initial Calibration

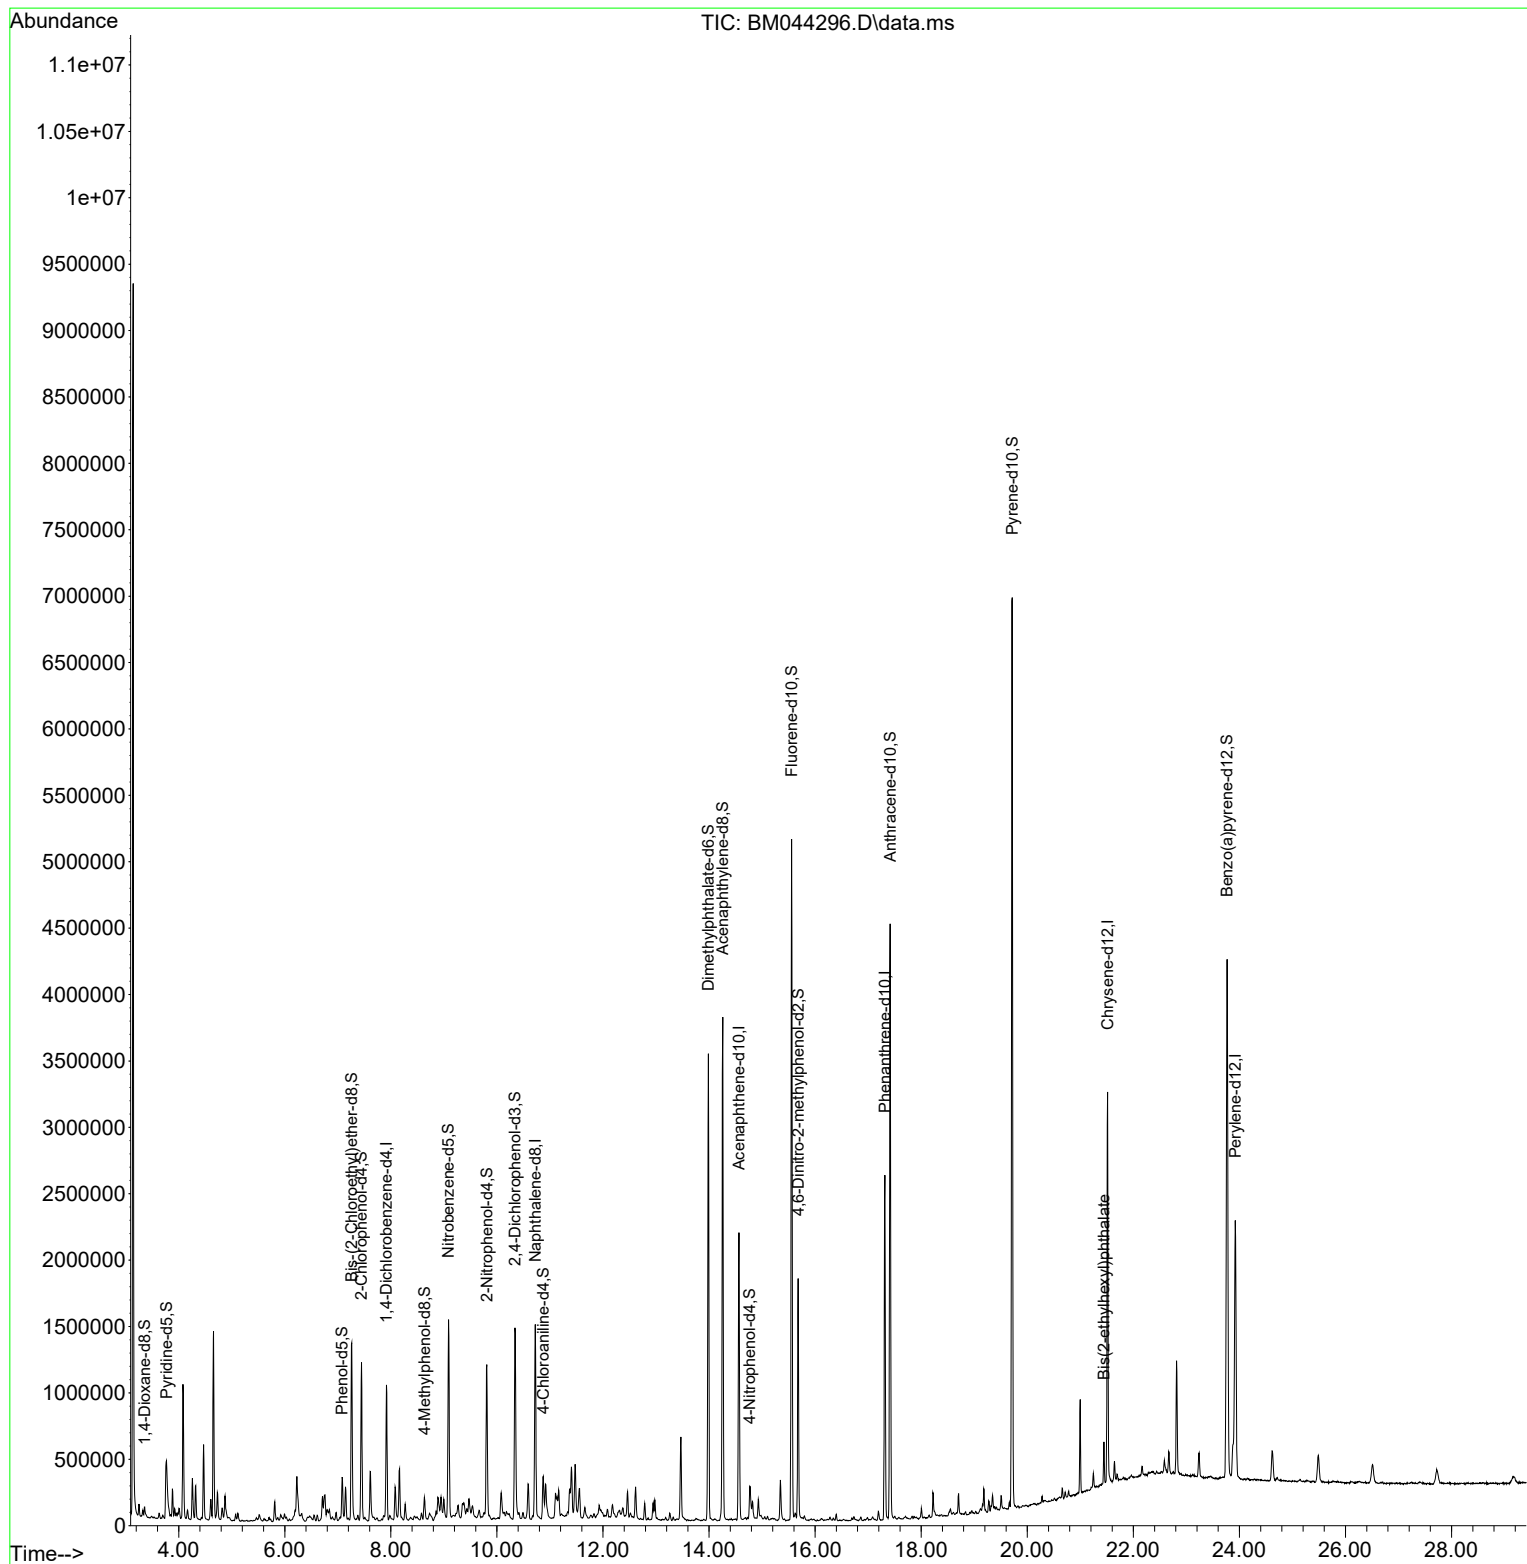

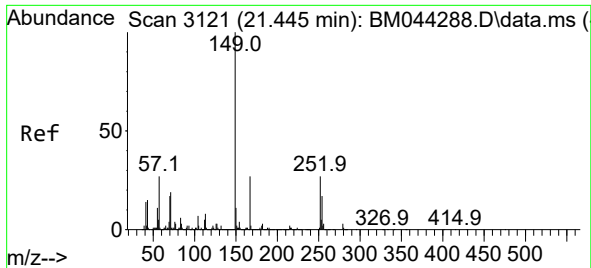

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.453 ng/ul
 RT: 21.445 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BM044296.D
 Acq: 24 Feb 2024 15:40

Instrument :
 BNA_M
 ClientSampleId :
 BH3Z7

Tgt Ion:149 Resp: 102369
 Ion Ratio Lower Upper
 149 100
 167 27.1 22.1 33.1
 279 3.4 2.4 3.6

