

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
 Data File : BM044297.D
 Acq On : 24 Feb 2024 16:17
 Operator : MA/JU
 Sample : P1494-22
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH400

Quant Time: Feb 25 23:00:45 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Feb 25 22:57:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.916	152	214336	20.000	ng/ul	0.00
20) Naphthalene-d8	10.722	136	931443	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.563	164	546646	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.315	188	1155637	20.000	ng/ul	0.00
79) Chrysene-d12	21.515	240	1021146	20.000	ng/ul	0.00
88) Perylene-d12	23.921	264	1101135	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	29674	4.368	ng/uL	0.00
4) Pyridine-d5	3.769	84	357016	19.243	ng/ul	0.00
7) Phenol-d5	7.081	99	153828	7.492	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	547453	41.173	ng/ul	0.00
11) 2-Chlorophenol-d4	7.445	132	464182	30.016	ng/ul	0.00
15) 4-Methylphenol-d8	8.634	113	35332	2.274	ng/ul	0.00
21) Nitrobenzene-d5	9.087	128	329993	43.573	ng/ul	0.00
24) 2-Nitrophenol-d4	9.810	143	346248	44.812	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.345	165	408226	29.951	ng/ul	0.00
31) 4-Chloroaniline-d4	10.875	131	247463	10.810	ng/ul	0.01
46) Dimethylphthalate-d6	13.986	166	1917168	45.474	ng/ul	0.00
49) Acenaphthylene-d8	14.257	160	2097669	43.245	ng/ul	0.00
54) 4-Nitrophenol-d4	14.769	143	58364	6.957	ng/ul	0.00
60) Fluorene-d10	15.557	176	1666359	46.698	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.680	200	273643	38.162	ng/ul	0.00
73) Anthracene-d10	17.415	188	2030152	36.843	ng/ul	0.00
81) Pyrene-d10	19.715	212	3056386	49.751	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.768	264	2305460	40.860	ng/ul	0.00


Target Compounds					Qvalue
86) Bis(2-ethylhexyl)phtha...	21.445	149	86563	1.629 ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044297.D
Acq On : 24 Feb 2024 16:17
Operator : MA/JU
Sample : P1494-22
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH400

Quant Time: Feb 25 23:00:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Feb 25 22:57:38 2024
Response via : Initial Calibration

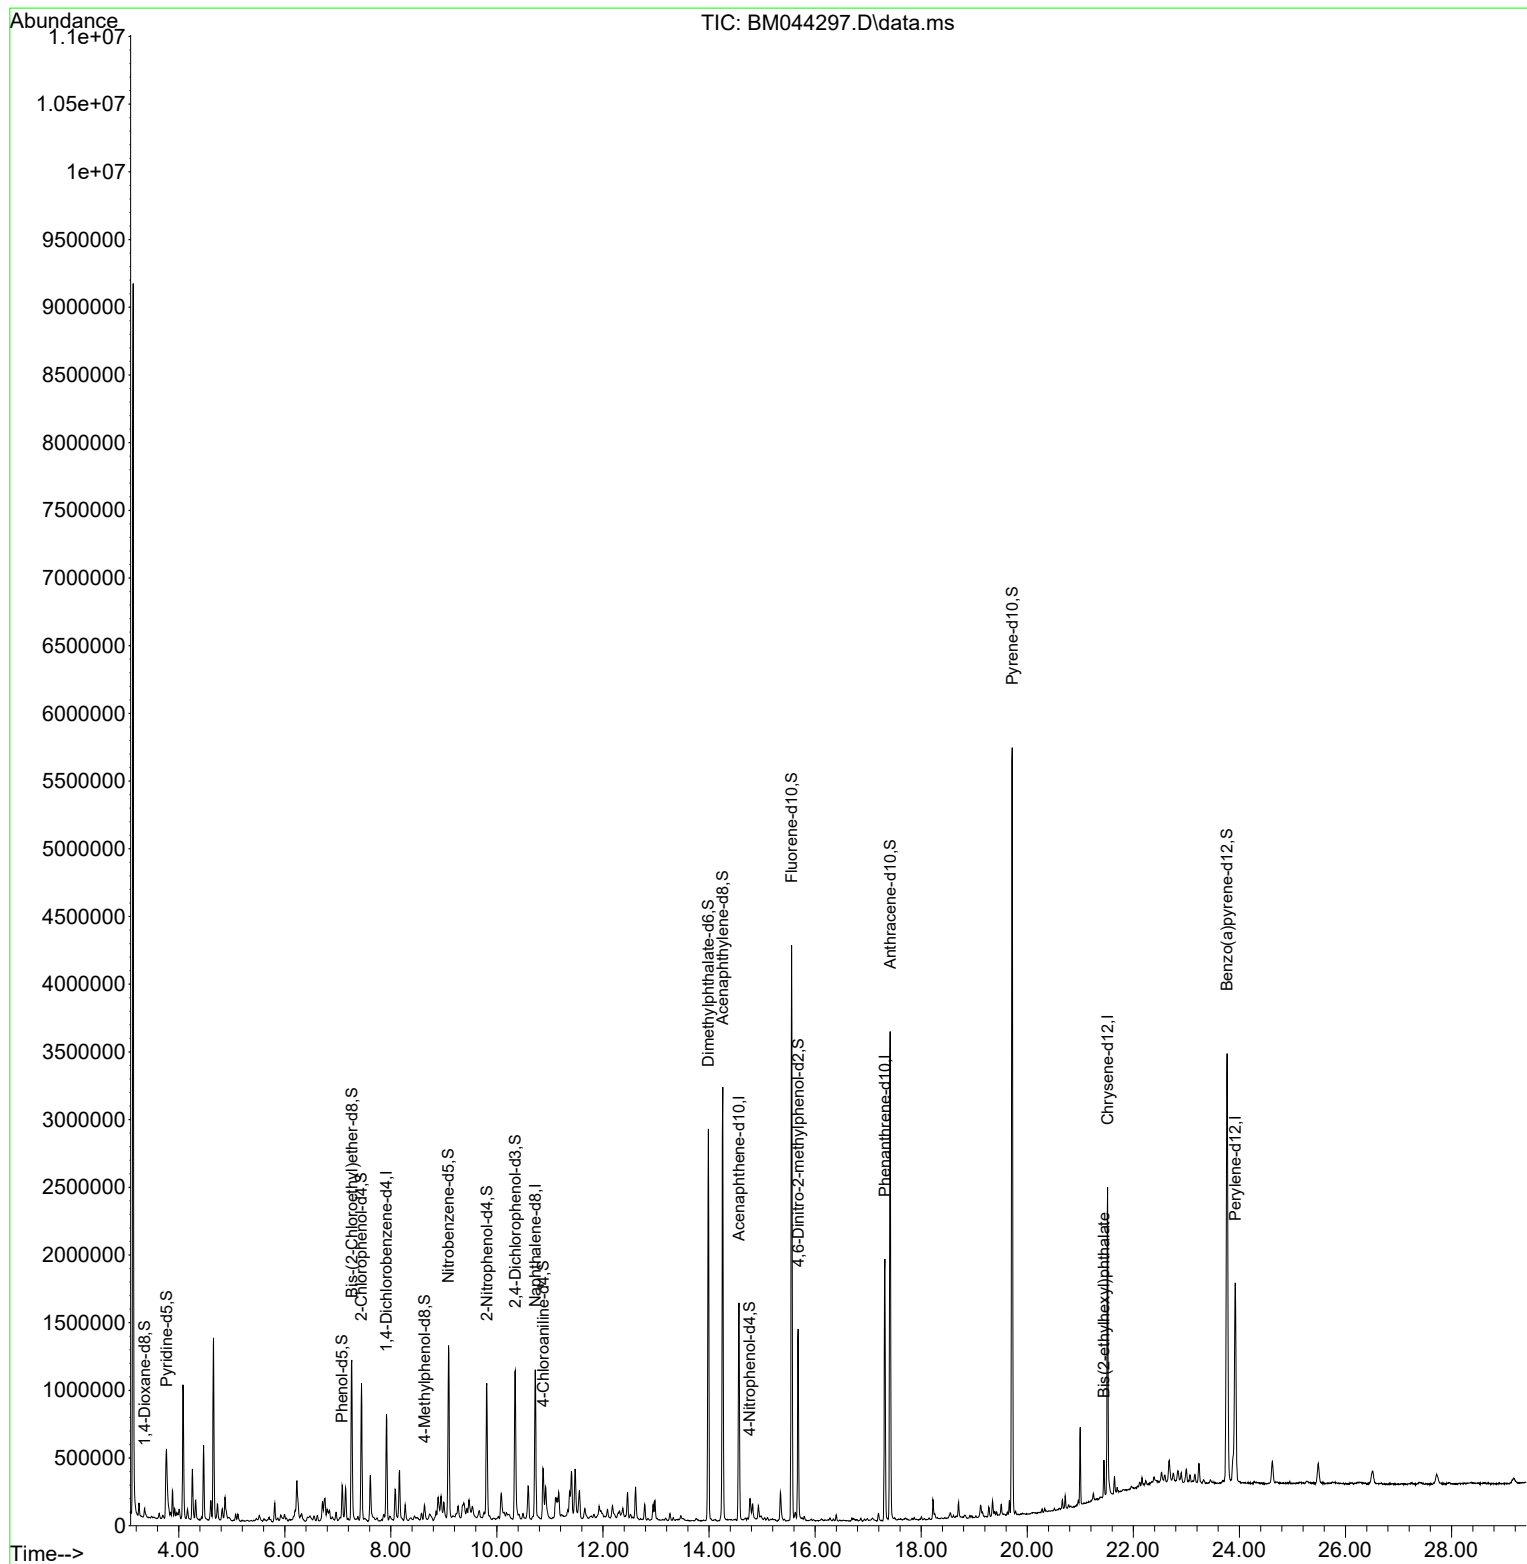

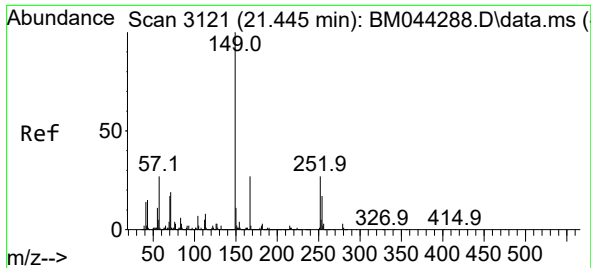

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.629 ng/ul
 RT: 21.445 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BM044297.D
 Acq: 24 Feb 2024 16:17

Instrument :
 BNA_M
 ClientSampleId :
 BH400

Tgt Ion:149 Resp: 86563
 Ion Ratio Lower Upper
 149 100
 167 26.3 22.1 33.1
 279 3.6 2.4 3.6

