

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
 Data File : BM044299.D
 Acq On : 24 Feb 2024 17:29
 Operator : MA/JU
 Sample : P1498-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB6

Quant Time: Feb 25 23:01:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Feb 25 22:57:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.916	152	216723	20.000	ng/ul	0.00
20) Naphthalene-d8	10.722	136	951791	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.563	164	574854	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.315	188	1227563	20.000	ng/ul	0.00
79) Chrysene-d12	21.515	240	1087325	20.000	ng/ul	0.00
88) Perylene-d12	23.921	264	1155195	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	27286	3.972	ng/uL	0.00
4) Pyridine-d5	3.769	84	338799	18.060	ng/ul	0.00
7) Phenol-d5	7.081	99	139952	6.741	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.257	67	432116	32.141	ng/ul	0.00
11) 2-Chlorophenol-d4	7.445	132	377374	24.134	ng/ul	0.00
15) 4-Methylphenol-d8	8.634	113	34667	2.207	ng/ul	0.00
21) Nitrobenzene-d5	9.087	128	257803	33.313	ng/ul	0.00
24) 2-Nitrophenol-d4	9.810	143	272078	34.460	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.345	165	330936	23.761	ng/ul	0.00
31) 4-Chloroaniline-d4	10.875	131	148430	6.346	ng/ul	0.01
46) Dimethylphthalate-d6	13.986	166	1571735	35.451	ng/ul	0.00
49) Acenaphthylene-d8	14.257	160	1719776	33.715	ng/ul	0.00
54) 4-Nitrophenol-d4	14.774	143	54373	6.163	ng/ul	0.01
60) Fluorene-d10	15.557	176	1351323	36.011	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.680	200	208624	27.390	ng/ul	0.00
73) Anthracene-d10	17.415	188	1546116	26.415	ng/ul	0.00
81) Pyrene-d10	19.709	212	2372075	36.262	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.768	264	1586906	26.809	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.445	149	75515	1.335	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044299.D
Acq On : 24 Feb 2024 17:29
Operator : MA/JU
Sample : P1498-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB6

Quant Time: Feb 25 23:01:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Feb 25 22:57:38 2024
Response via : Initial Calibration

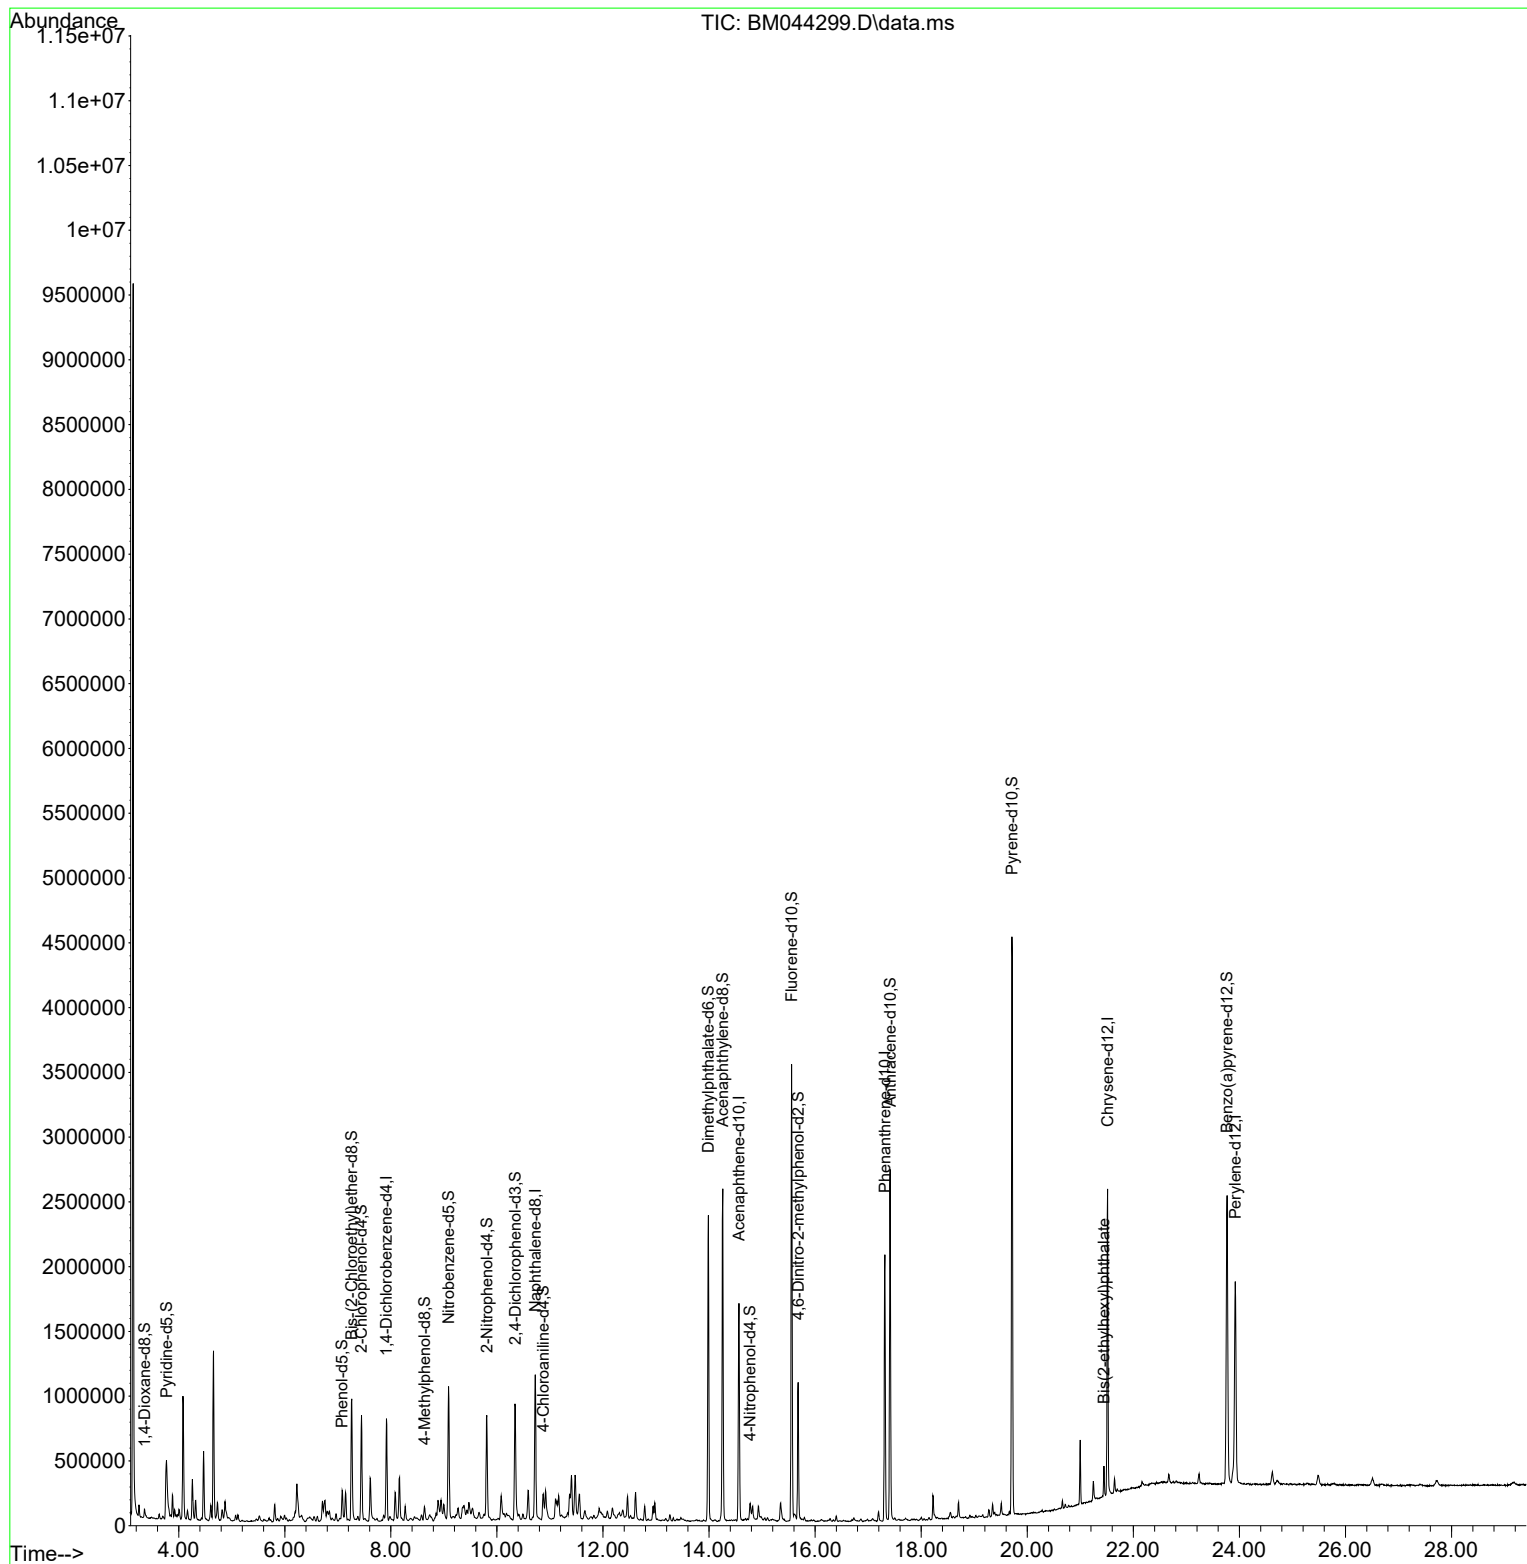

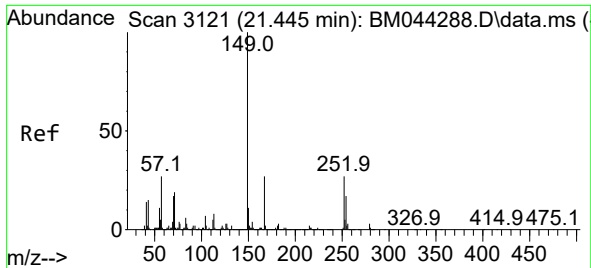

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.335 ng/ul
 RT: 21.445 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BM044299.D
 Acq: 24 Feb 2024 17:29

Instrument :
 BNA_M
 ClientSampleId :
 C0AB6

Tgt Ion:149 Resp: 75515
 Ion Ratio Lower Upper
 149 100
 167 28.3 22.1 33.1
 279 3.4 2.4 3.6

