

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
 Data File : BM044309.D
 Acq On : 25 Feb 2024 00:09
 Operator : MA/JU
 Sample : P1494-17
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3X2

Quant Time: Feb 25 23:04:45 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Feb 25 22:57:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	166259	20.000	ng/ul	0.00
20) Naphthalene-d8	10.727	136	714333	20.000	ng/ul	0.01
38) Acenaphthene-d10	14.568	164	417280	20.000	ng/ul	0.01
64) Phenanthrene-d10	17.315	188	910011	20.000	ng/ul	0.00
79) Chrysene-d12	21.515	240	834417	20.000	ng/ul	0.00
88) Perylene-d12	23.927	264	952451	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.357	96	26591	5.046	ng/uL	0.00
4) Pyridine-d5	3.781	84	153856	10.691	ng/ul	0.01
7) Phenol-d5	7.086	99	151251	9.496	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	471032	45.670	ng/ul	0.00
11) 2-Chlorophenol-d4	7.451	132	442938	36.925	ng/ul	0.01
15) 4-Methylphenol-d8	8.633	113	262267	21.763	ng/ul	0.00
21) Nitrobenzene-d5	9.092	128	278018	47.867	ng/ul	0.00
24) 2-Nitrophenol-d4	9.816	143	280686	47.368	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	10.345	165	433760	41.497	ng/ul	0.00
31) 4-Chloroaniline-d4	10.874	131	629921	35.882	ng/ul	0.01
46) Dimethylphthalate-d6	13.992	166	1558076	48.414	ng/ul	0.01
49) Acenaphthylene-d8	14.262	160	1805064	48.749	ng/ul	0.01
54) 4-Nitrophenol-d4	14.780	143	39267	6.132	ng/ul	0.02
60) Fluorene-d10	15.562	176	1379096	50.629	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.686	200	234030	41.447	ng/ul	0.00
73) Anthracene-d10	17.415	188	2267155	52.250	ng/ul	0.00
81) Pyrene-d10	19.715	212	2671004	53.208	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.774	264	2633622	53.963	ng/ul	0.01
Target Compounds						
					Qvalue	
48) 2,6-Dinitrotoluene	13.992	165	8305	1.350	ng/ul#	30


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044309.D
Acq On : 25 Feb 2024 00:09
Operator : MA/JU
Sample : P1494-17
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3X2


Quant Time: Feb 25 23:04:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Feb 25 22:57:38 2024
Response via : Initial Calibration

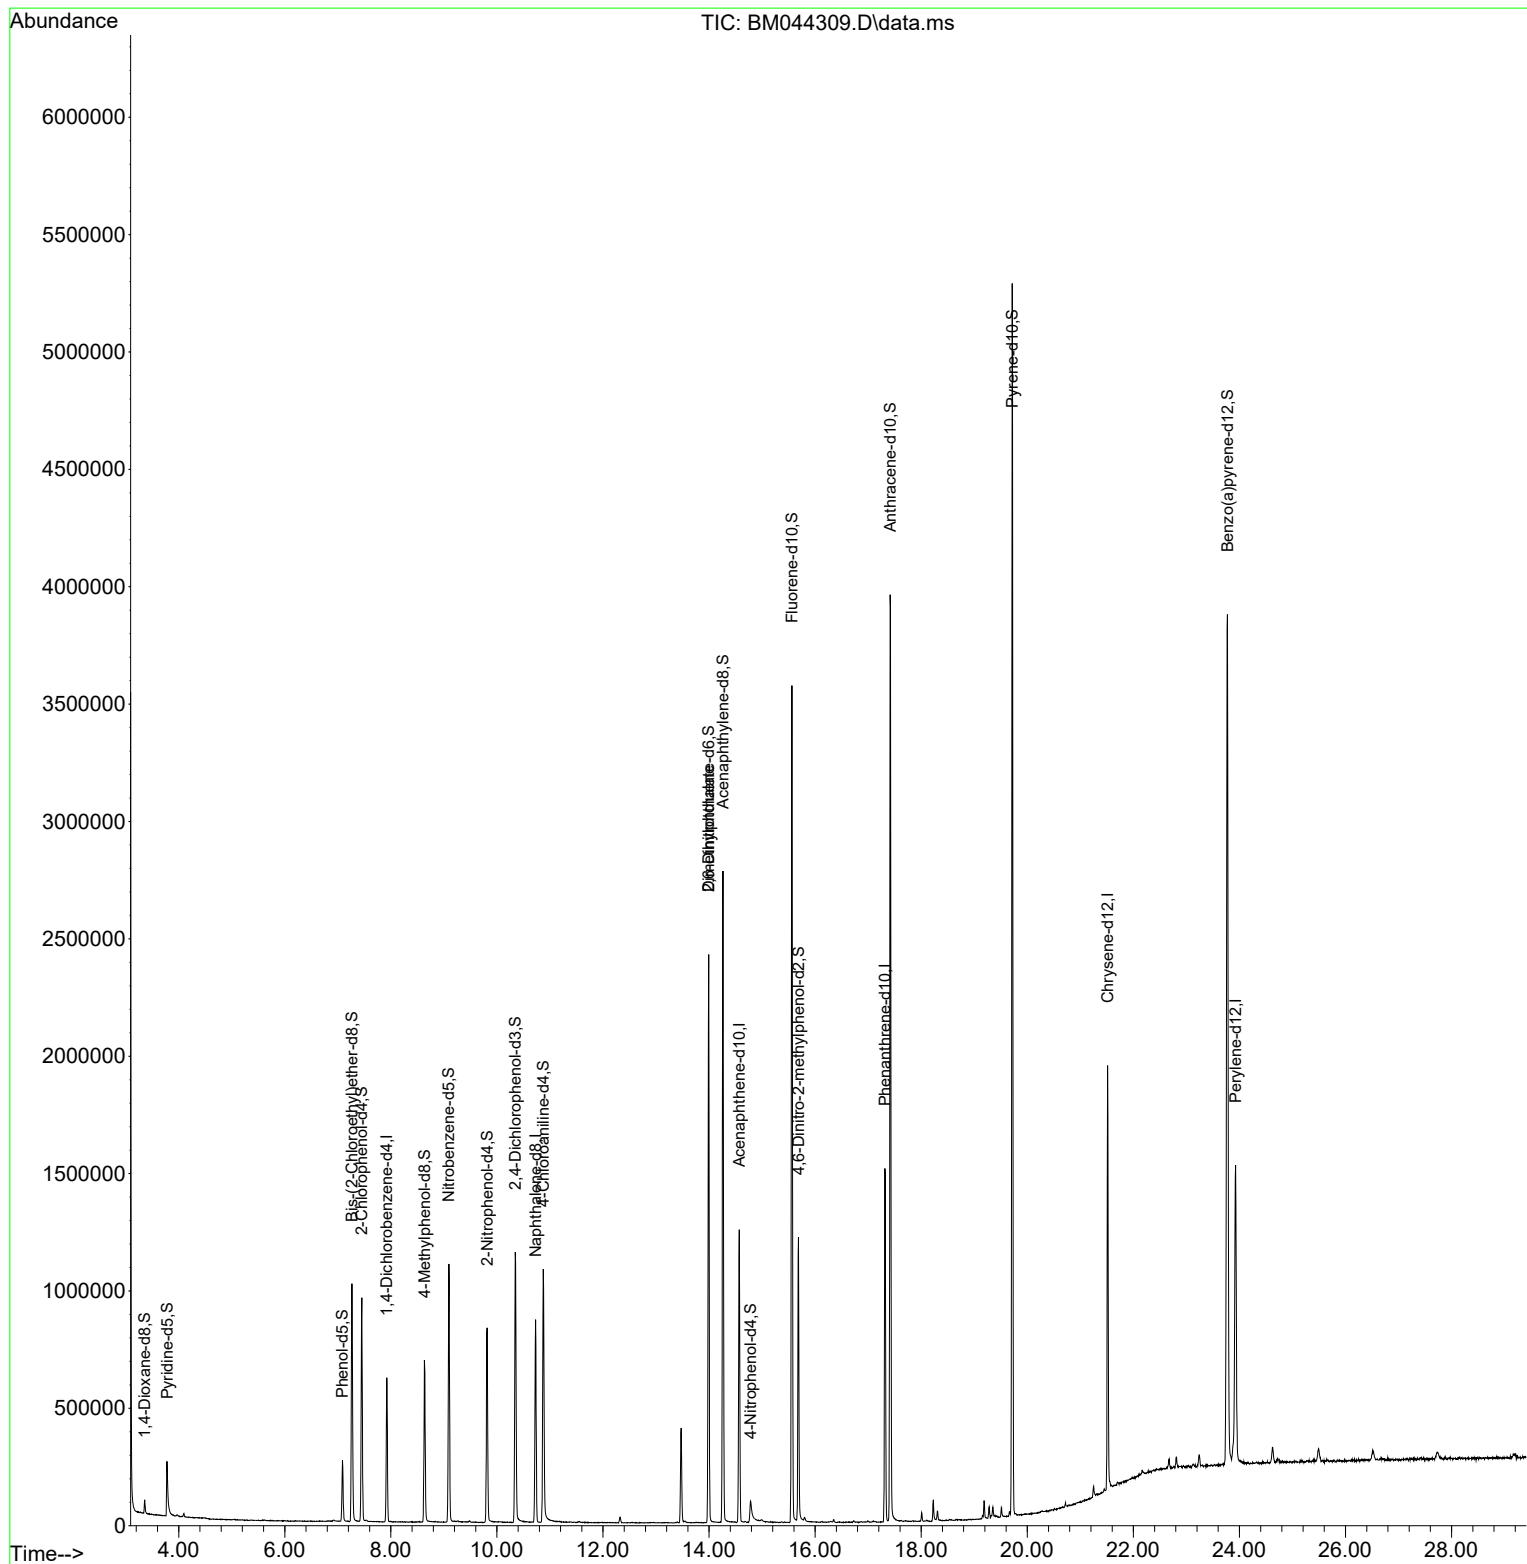

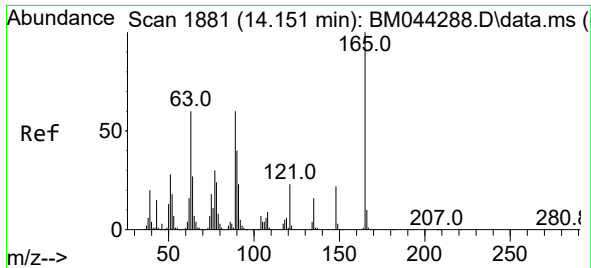

#48
 2,6-Dinitrotoluene
 Concen: 1.350 ng/ul
 RT: 13.992 min Scan# 11
 Delta R.T. -0.159 min
 Lab File: BM044309.D
 Acq: 25 Feb 2024 00:09

Instrument :
 BNA_M
 ClientSampleId :
 BH3X2

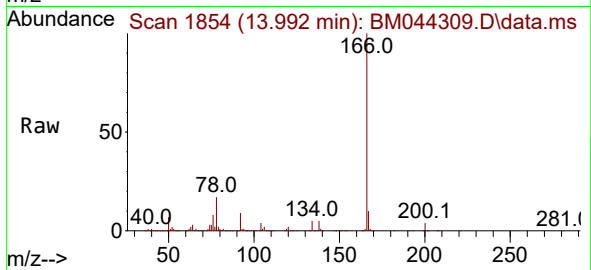

Tgt Ion:165 Resp: 8305
 Ion Ratio Lower Upper
 165 100
 89 0.0 48.2 72.2#
 121 45.1 18.7 28.1#

