

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
 Data File : BM044313.D
 Acq On : 25 Feb 2024 02:34
 Operator : MA/JU
 Sample : P1494-20
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3X7

Quant Time: Feb 25 23:05:23 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Feb 25 22:57:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	204920	20.000	ng/ul	0.00
20) Naphthalene-d8	10.727	136	897787	20.000	ng/ul	0.01
38) Acenaphthene-d10	14.563	164	536811	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.315	188	1147036	20.000	ng/ul	0.00
79) Chrysene-d12	21.515	240	1019126	20.000	ng/ul	0.00
88) Perylene-d12	23.921	264	1078701	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.357	96	27159	4.182	ng/uL	0.00
4) Pyridine-d5	3.775	84	276657	15.597	ng/ul	0.00
7) Phenol-d5	7.087	99	139288	7.095	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	425790	33.495	ng/ul	0.00
11) 2-Chlorophenol-d4	7.451	132	383602	25.945	ng/ul	0.01
15) 4-Methylphenol-d8	8.639	113	36345	2.447	ng/ul	0.01
21) Nitrobenzene-d5	9.092	128	259383	35.533	ng/ul	0.00
24) 2-Nitrophenol-d4	9.810	143	272924	36.646	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.345	165	353216	26.886	ng/ul	0.00
31) 4-Chloroaniline-d4	10.875	131	176114	7.982	ng/ul	0.01
46) Dimethylphthalate-d6	13.992	166	1707992	41.255	ng/ul	0.01
49) Acenaphthylene-d8	14.257	160	1750379	36.746	ng/ul	0.00
54) 4-Nitrophenol-d4	14.774	143	62636	7.603	ng/ul	0.01
60) Fluorene-d10	15.562	176	1448425	41.334	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.686	200	265389	37.289	ng/ul	0.00
73) Anthracene-d10	17.415	188	2001076	36.588	ng/ul	0.00
81) Pyrene-d10	19.715	212	2973249	48.494	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.768	264	2147224	38.847	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.444	149	75722	1.428	ng/ul	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044313.D
Acq On : 25 Feb 2024 02:34
Operator : MA/JU
Sample : P1494-20
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3X7

Quant Time: Feb 25 23:05:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Feb 25 22:57:38 2024
Response via : Initial Calibration

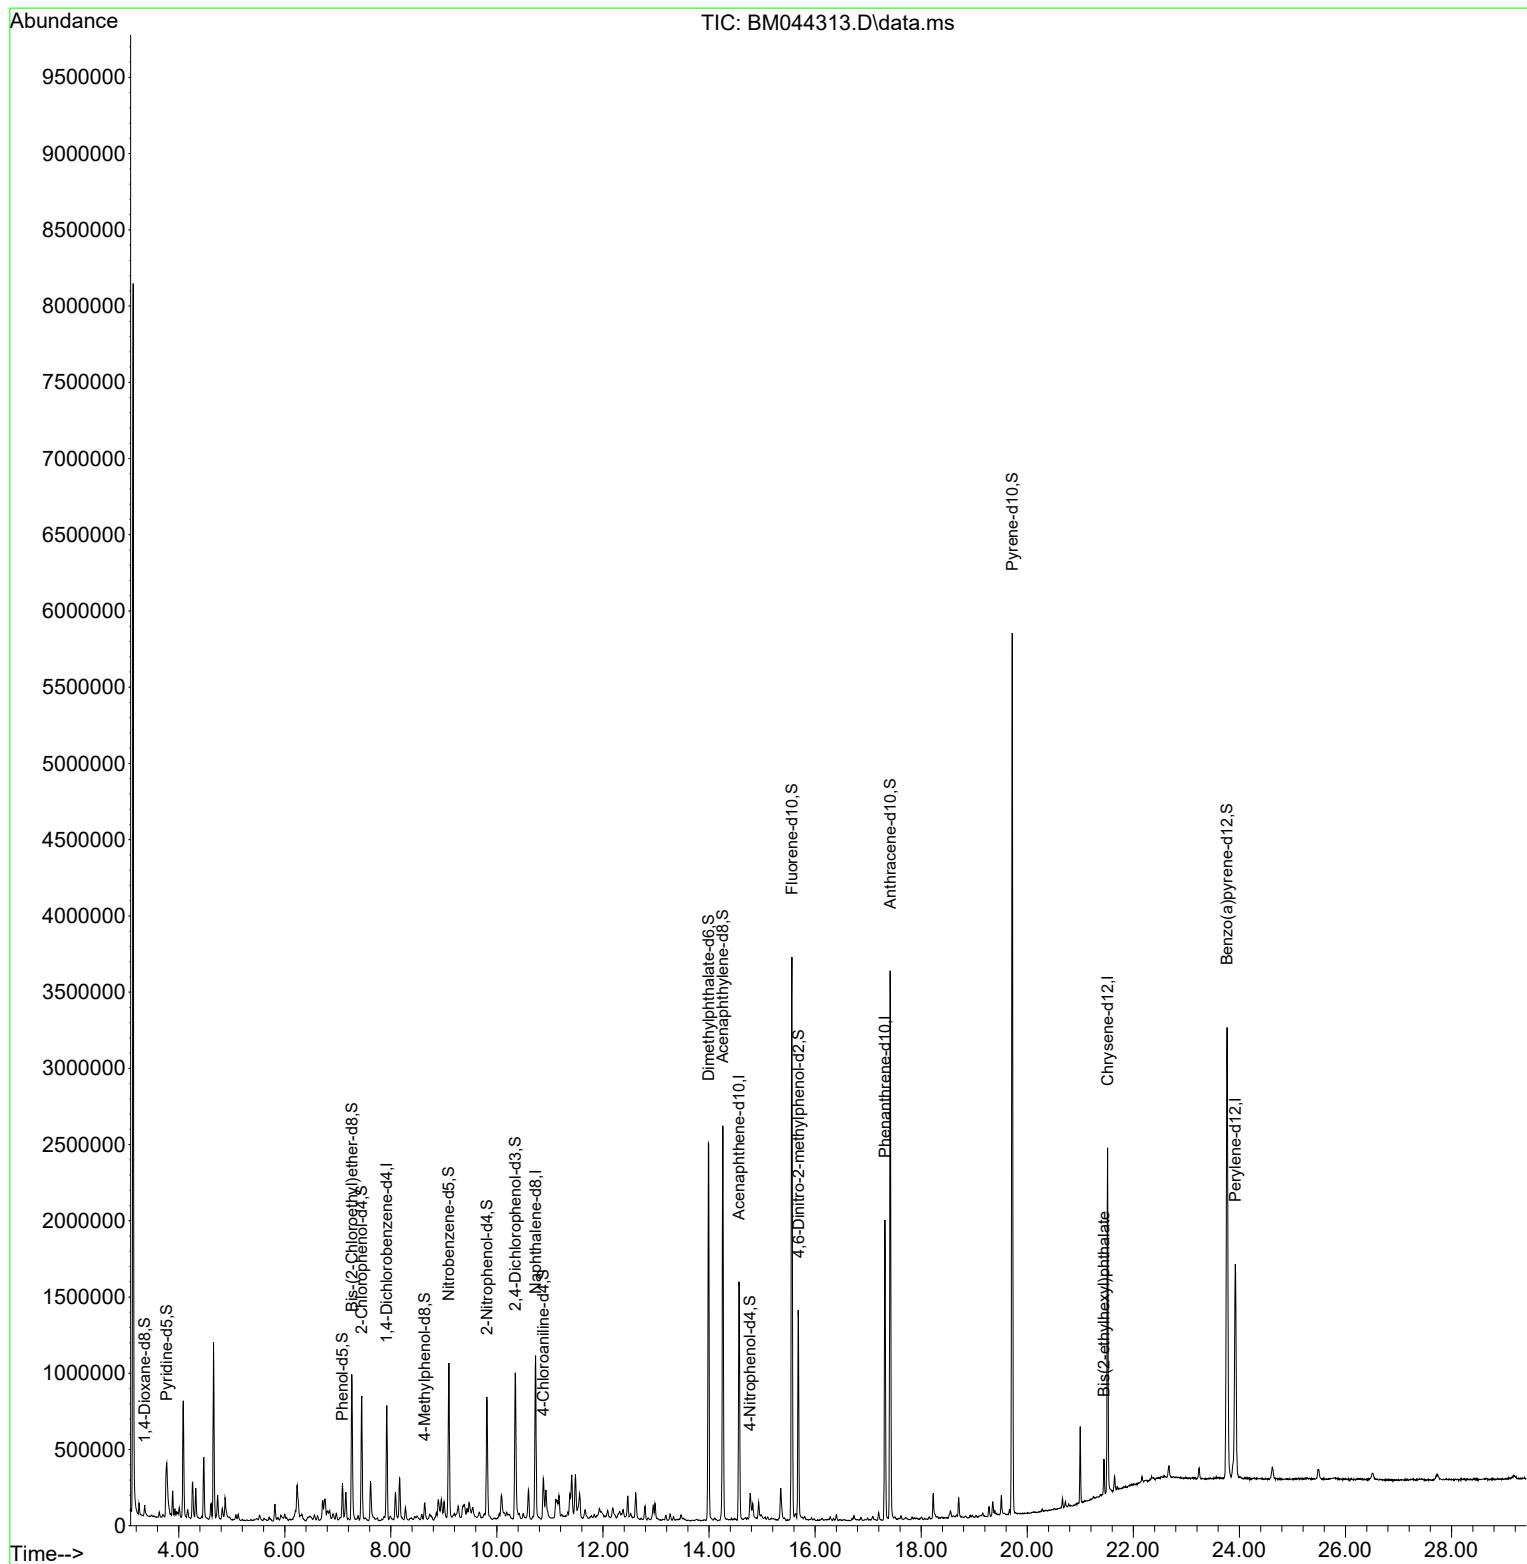

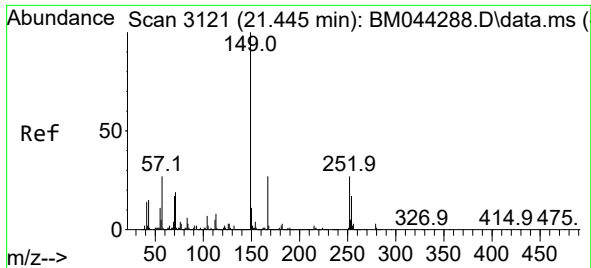

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.428 ng/ul
 RT: 21.444 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BM044313.D
 Acq: 25 Feb 2024 02:34

Instrument :
 BNA_M
 ClientSampleId :
 BH3X7

Tgt Ion:149 Resp: 75722
 Ion Ratio Lower Upper
 149 100
 167 27.7 22.1 33.1
 279 3.1 2.4 3.6

