




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044293.D
Acq On : 24 Feb 2024 13:51
Operator : MA/JU
Sample : P1498-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE2

Manual IntegrationsAPPROVED

Quant Time: Feb 25 23:00:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Feb 25 22:57:38 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/26/2024
Supervised By :mohammad ahmed 02/26/2024

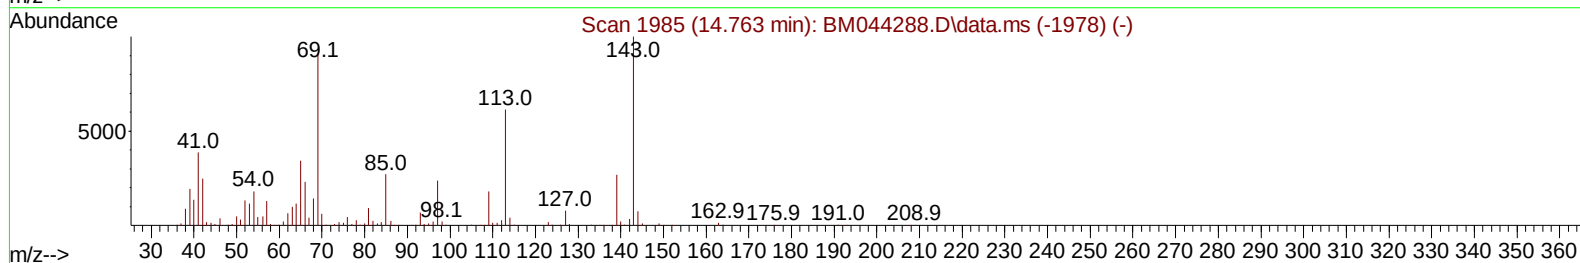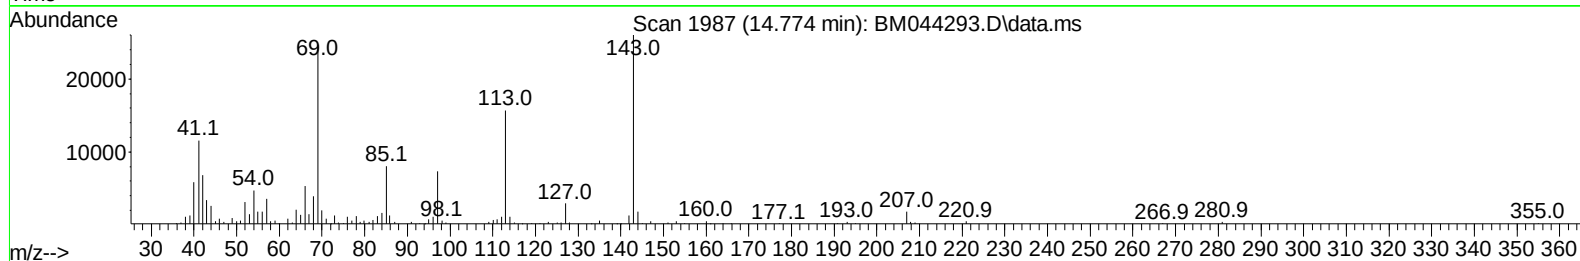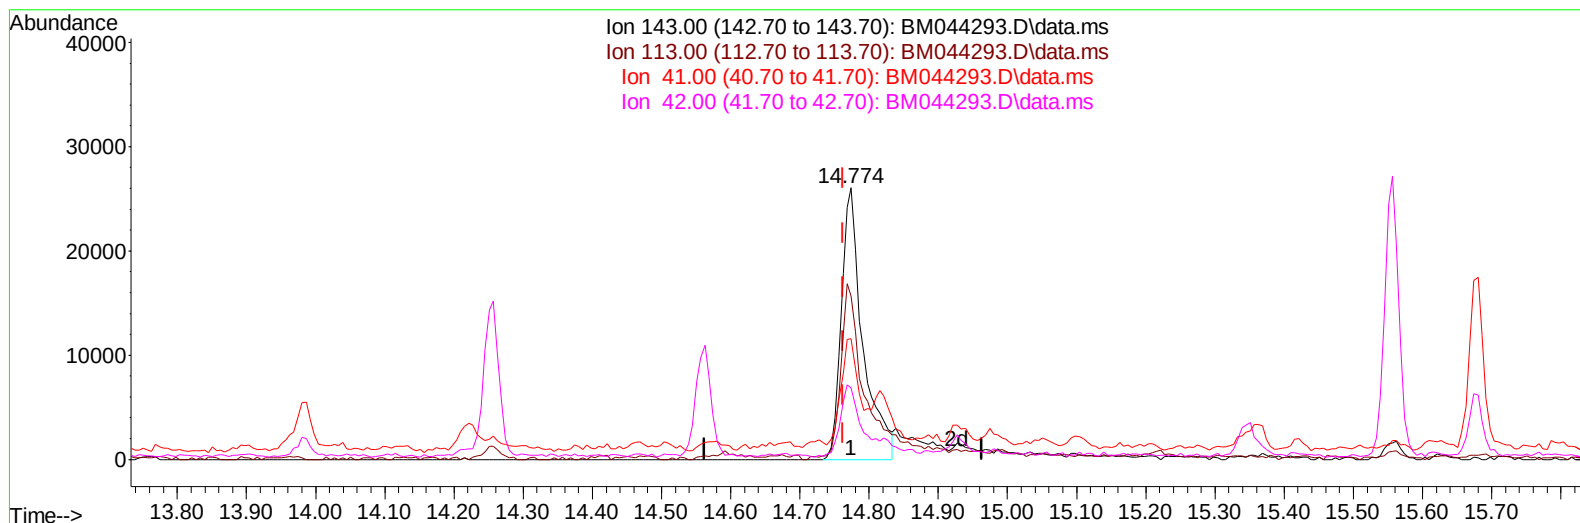

TIC: BM044293.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.774min (+ 0.012) 6.31 ng/ul

response 55990

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	59.00	60.35
41.00	38.20	44.41
42.00	25.30	26.25




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044293.D
Acq On : 24 Feb 2024 13:51
Operator : MA/JU
Sample : P1498-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE2

Manual IntegrationsAPPROVED

Quant Time: Feb 25 23:00:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Feb 25 22:57:38 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/26/2024
Supervised By :mohammad ahmed 02/26/2024

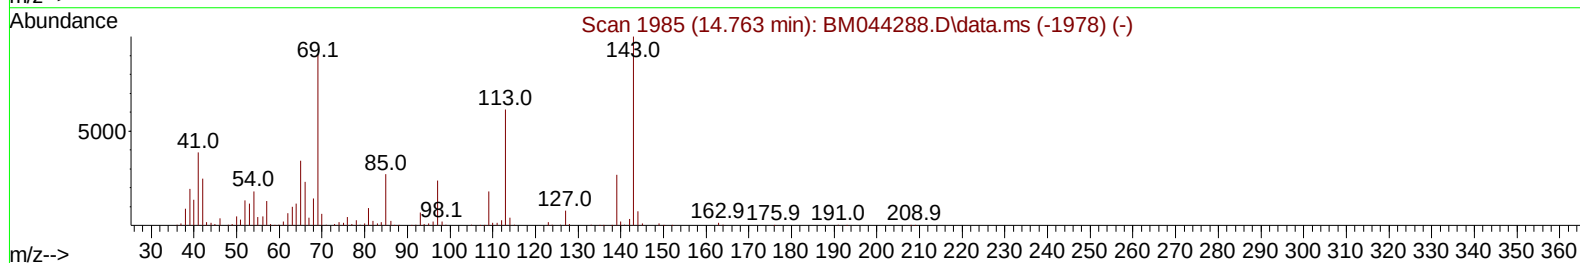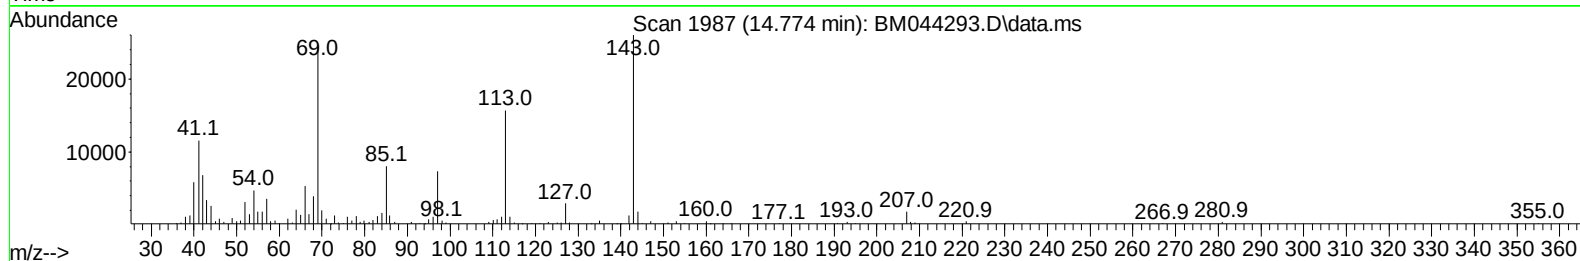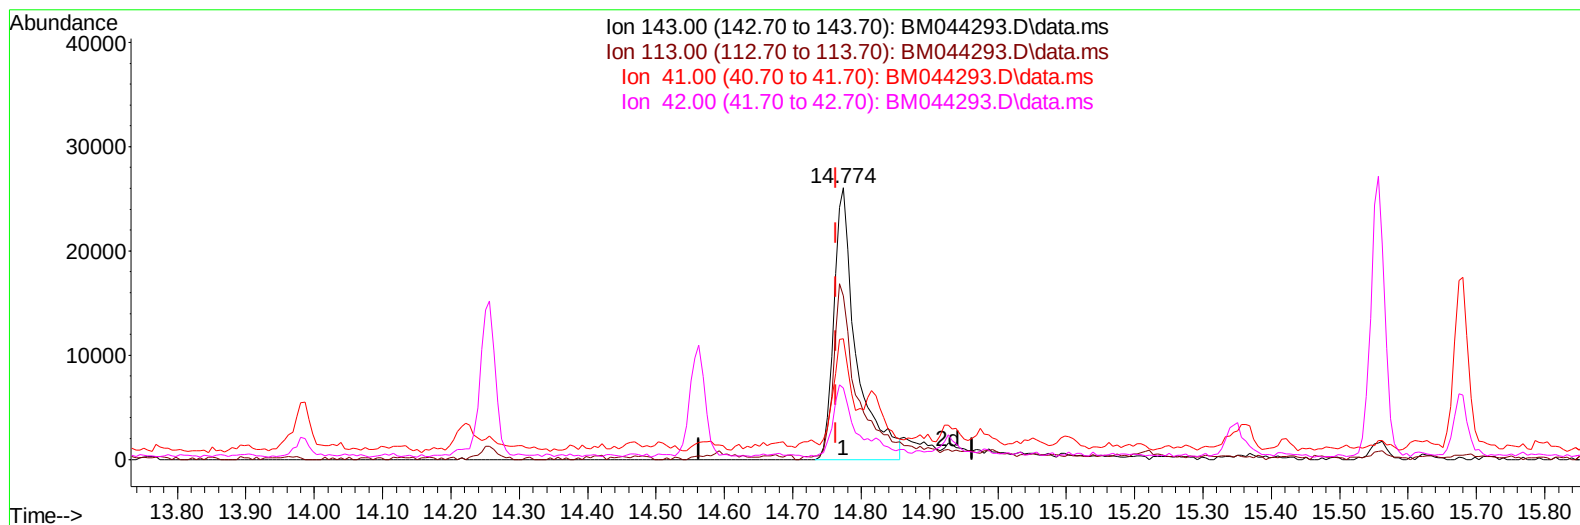

TIC: BM044293.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.774min (+ 0.012) 6.68 ng/ul m

response 59243

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	59.00	60.35
41.00	38.20	44.41
42.00	25.30	26.25

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
 Data File : BM044293.D
 Acq On : 24 Feb 2024 13:51
 Operator : MA/JU
 Sample : P1498-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 02/26/2024
 Supervised By :mohammad ahmed 02/26/2024

Quant Time: Feb 25 23:36:45 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Feb 25 22:57:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.916	152	225607	20.000	ng/ul	0.00
20) Naphthalene-d8	10.722	136	976062	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.563	164	578266	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.315	188	1209157	20.000	ng/ul	0.00
79) Chrysene-d12	21.509	240	1076791	20.000	ng/ul	0.00
88) Perylene-d12	23.921	264	1151177	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.357	96	32864	4.596	ng/uL	0.00
4) Pyridine-d5	3.769	84	379733	19.445	ng/ul	0.00
7) Phenol-d5	7.081	99	181066	8.378	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.257	67	547975	39.154	ng/ul	0.00
11) 2-Chlorophenol-d4	7.445	132	497930	30.590	ng/ul	0.00
15) 4-Methylphenol-d8	8.628	113	64757	3.960	ng/ul	0.00
21) Nitrobenzene-d5	9.086	128	326715	41.168	ng/ul	0.00
24) 2-Nitrophenol-d4	9.804	143	336030	41.501	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.339	165	453721	31.767	ng/ul	0.00
31) 4-Chloroaniline-d4	10.869	131	206314	8.601	ng/ul	0.00
46) Dimethylphthalate-d6	13.986	166	1889964	42.377	ng/ul	0.00
49) Acenaphthylene-d8	14.257	160	2070586	40.352	ng/ul	0.00
54) 4-Nitrophenol-d4	14.774	143	59243m	6.676	ng/ul	0.01
60) Fluorene-d10	15.557	176	1628193	43.133	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.680	200	247842	33.034	ng/ul	0.00
73) Anthracene-d10	17.415	188	1937578	33.607	ng/ul	0.00
81) Pyrene-d10	19.709	212	2853779	44.053	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.768	264	2103384	35.658	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.444	149	77598	1.385	ng/ul#	Qvalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044293.D
Acq On : 24 Feb 2024 13:51
Operator : MA/JU
Sample : P1498-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE2

Manual IntegrationsAPPROVED

Quant Time: Feb 25 23:36:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Feb 25 22:57:38 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/26/2024
Supervised By :mohammad ahmed 02/26/2024

