

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
 Data File : BM044295.D
 Acq On : 24 Feb 2024 15:04
 Operator : MA/JU
 Sample : P1498-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE8

Quant Time: Feb 25 23:54:56 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Feb 25 22:57:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.916	152	249084	20.000	ng/u1	0.00
20) Naphthalene-d8	10.722	136	1077845	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.563	164	632048	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.315	188	1341327	20.000	ng/u1	0.00
79) Chrysene-d12	21.515	240	1173322	20.000	ng/u1	0.00
88) Perylene-d12	23.921	264	1228475	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	42876	5.431	ng/uL	0.00
4) Pyridine-d5	3.769	84	404091	18.742	ng/u1	0.00
7) Phenol-d5	7.081	99	202062	8.468	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.257	67	574848	37.203	ng/u1	0.00
11) 2-Chlorophenol-d4	7.445	132	524149	29.166	ng/u1	0.00
15) 4-Methylphenol-d8	8.634	113	59538	3.298	ng/u1	0.00
21) Nitrobenzene-d5	9.087	128	347287	39.628	ng/u1	0.00
24) 2-Nitrophenol-d4	9.810	143	361582	40.440	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.339	165	499572	31.674	ng/u1	0.00
31) 4-Chloroaniline-d4	10.875	131	154701	5.840	ng/u1	0.01
46) Dimethylphthalate-d6	13.986	166	2099688	43.074	ng/u1	0.00
49) Acenaphthylene-d8	14.257	160	2282878	40.704	ng/u1	0.00
54) 4-Nitrophenol-d4	14.774	143	80158	8.264	ng/u1	0.01
60) Fluorene-d10	15.557	176	1803865	43.721	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.680	200	302076	36.295	ng/u1	0.00
73) Anthracene-d10	17.415	188	2095847	32.770	ng/u1	0.00
81) Pyrene-d10	19.709	212	3237217	45.860	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.768	264	2177144	34.586	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.393	88	27701	3.329	ng/uL#	86
86) Bis(2-ethylhexyl)phtha...	21.445	149	107331	1.758	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044295.D
Acq On : 24 Feb 2024 15:04
Operator : MA/JU
Sample : P1498-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE8

Quant Time: Feb 25 23:54:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Feb 25 22:57:38 2024
Response via : Initial Calibration




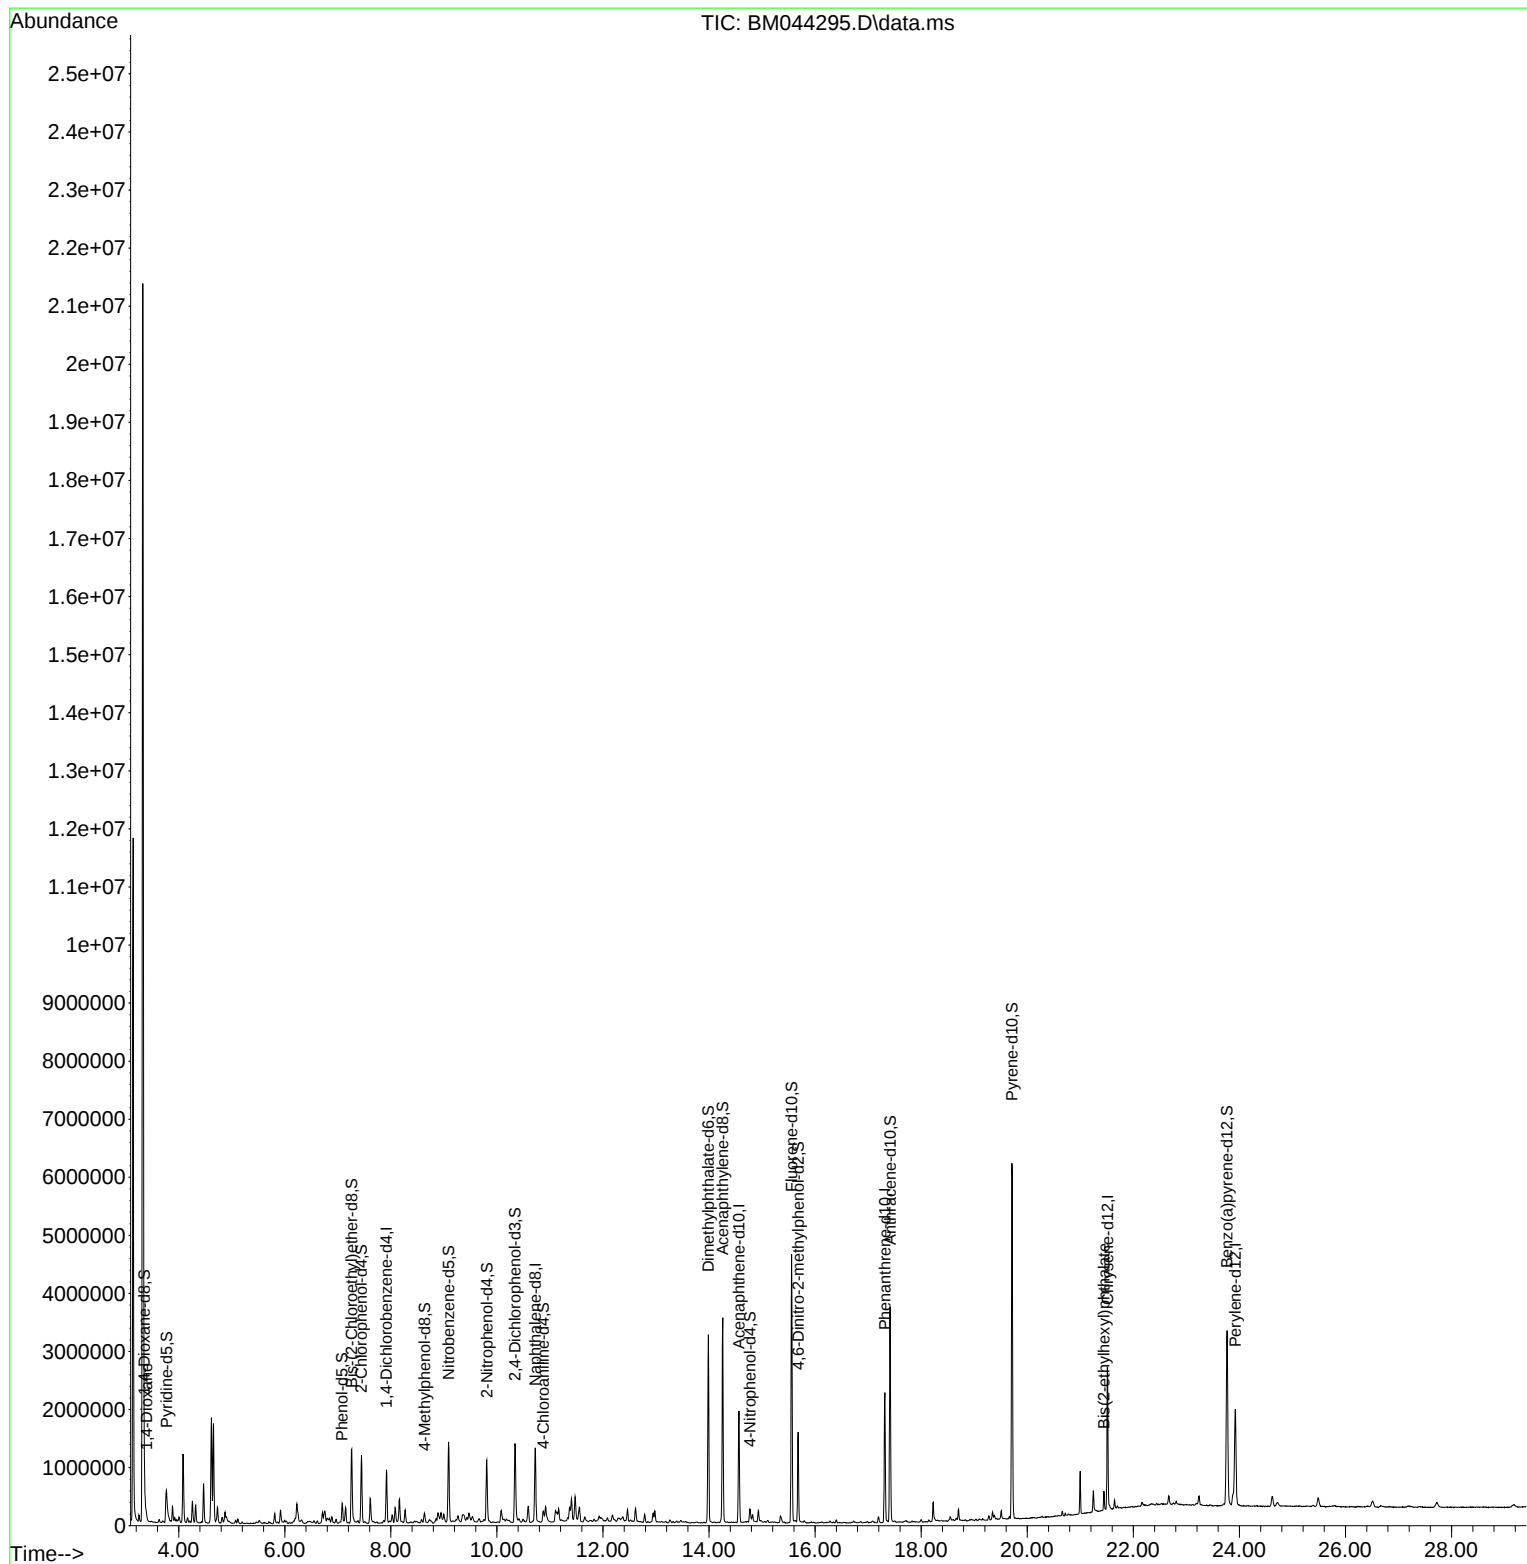


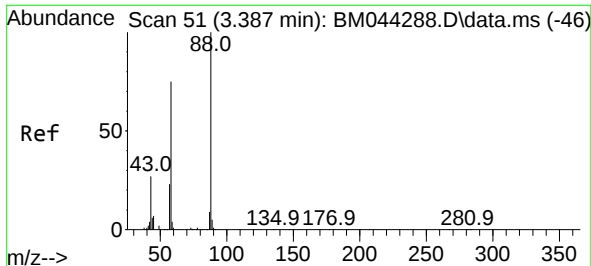

#2
1,4-Dioxane
Concen: 3.329 ng/uL
RT: 3.393 min Scan# 51
Delta R.T. 0.006 min
Lab File: BM044295.D
Acq: 24 Feb 2024 15:04

Instrument :
BNA_M
ClientSampleId :
C0AE8

Tgt Ion: 88 Resp: 27701
Ion Ratio Lower Upper
88 100
43 48.1 21.2 31.8#
58 75.9 58.3 87.5

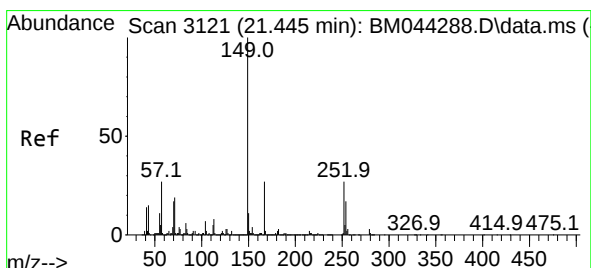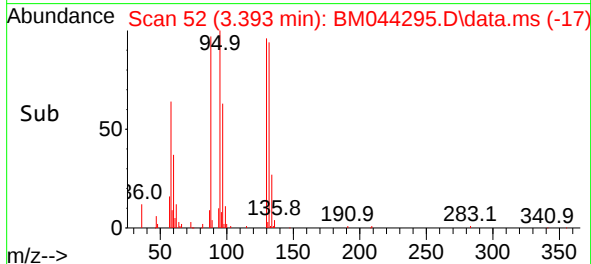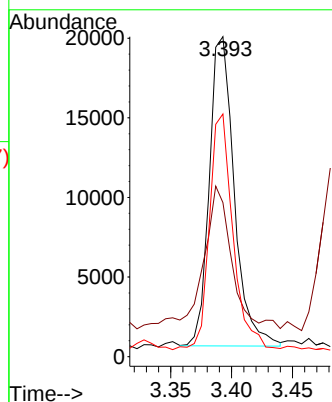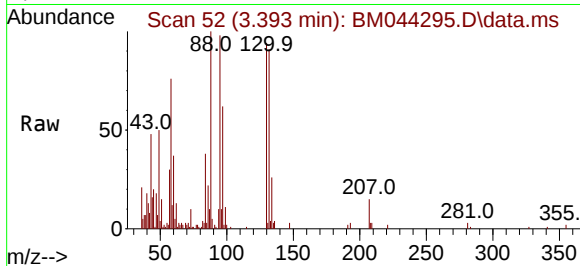

#86
Bis(2-ethylhexyl)phthalate
Concen: 1.758 ng/uL
RT: 21.445 min Scan# 3121
Delta R.T. -0.000 min
Lab File: BM044295.D
Acq: 24 Feb 2024 15:04

Tgt Ion:149 Resp: 107331
Ion Ratio Lower Upper
149 100
167 28.0 22.1 33.1
279 3.4 2.4 3.6

