

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM022424\  
 Data File : BM044299.D  
 Acq On : 24 Feb 2024 17:29  
 Operator : MA/JU  
 Sample : P1498-01  
 Misc :  
 ALS Vial : 21 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 C0AB6

Quant Time: Feb 26 00:27:27 2024  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM022324.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Sun Feb 25 22:57:38 2024  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc   | Units | Dev(Min)     |
|-------------------------------|--------|------|----------|--------|-------|--------------|
| -----                         |        |      |          |        |       |              |
| Internal Standards            |        |      |          |        |       |              |
| 1) 1,4-Dichlorobenzene-d4     | 7.916  | 152  | 216723   | 20.000 | ng/u1 | 0.00         |
| 20) Naphthalene-d8            | 10.722 | 136  | 951791   | 20.000 | ng/u1 | 0.00         |
| 38) Acenaphthene-d10          | 14.563 | 164  | 574854   | 20.000 | ng/u1 | 0.00         |
| 64) Phenanthrene-d10          | 17.315 | 188  | 1227563  | 20.000 | ng/u1 | 0.00         |
| 79) Chrysene-d12              | 21.515 | 240  | 1087325  | 20.000 | ng/u1 | 0.00         |
| 88) Perylene-d12              | 23.921 | 264  | 1155195  | 20.000 | ng/u1 | 0.00         |
| System Monitoring Compounds   |        |      |          |        |       |              |
| 3) 1,4-Dioxane-d8             | 3.358  | 96   | 27286    | 3.972  | ng/uL | 0.00         |
| 4) Pyridine-d5                | 3.769  | 84   | 338799   | 18.060 | ng/u1 | 0.00         |
| 7) Phenol-d5                  | 7.081  | 99   | 139952   | 6.741  | ng/u1 | 0.00         |
| 9) Bis-(2-Chloroethyl)eth...  | 7.257  | 67   | 432116   | 32.141 | ng/u1 | 0.00         |
| 11) 2-Chlorophenol-d4         | 7.445  | 132  | 377374   | 24.134 | ng/u1 | 0.00         |
| 15) 4-Methylphenol-d8         | 8.634  | 113  | 34667    | 2.207  | ng/u1 | 0.00         |
| 21) Nitrobenzene-d5           | 9.087  | 128  | 257803   | 33.313 | ng/u1 | 0.00         |
| 24) 2-Nitrophenol-d4          | 9.810  | 143  | 272078   | 34.460 | ng/u1 | 0.00         |
| 28) 2,4-Dichlorophenol-d3     | 10.345 | 165  | 330936   | 23.761 | ng/u1 | 0.00         |
| 31) 4-Chloroaniline-d4        | 10.875 | 131  | 148430   | 6.346  | ng/u1 | 0.01         |
| 46) Dimethylphthalate-d6      | 13.986 | 166  | 1571735  | 35.451 | ng/u1 | 0.00         |
| 49) Acenaphthylene-d8         | 14.257 | 160  | 1719776  | 33.715 | ng/u1 | 0.00         |
| 54) 4-Nitrophenol-d4          | 14.774 | 143  | 54373    | 6.163  | ng/u1 | 0.01         |
| 60) Fluorene-d10              | 15.557 | 176  | 1351323  | 36.011 | ng/u1 | 0.00         |
| 65) 4,6-Dinitro-2-methylph... | 15.680 | 200  | 208624   | 27.390 | ng/u1 | 0.00         |
| 73) Anthracene-d10            | 17.415 | 188  | 1546116  | 26.415 | ng/u1 | 0.00         |
| 81) Pyrene-d10                | 19.709 | 212  | 2372075  | 36.262 | ng/u1 | 0.00         |
| 92) Benzo(a)pyrene-d12        | 23.768 | 264  | 1586906  | 26.809 | ng/u1 | 0.00         |
| Target Compounds              |        |      |          |        |       |              |
| 86) Bis(2-ethylhexyl)phtha... | 21.445 | 149  | 75515    | 1.335  | ng/u1 | Qvalue<br>99 |
| -----                         |        |      |          |        |       |              |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM022424\  
Data File : BM044299.D  
Acq On : 24 Feb 2024 17:29  
Operator : MA/JU  
Sample : P1498-01  
Misc :  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
C0AB6

Quant Time: Feb 26 00:27:27 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM022324.MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Sun Feb 25 22:57:38 2024  
Response via : Initial Calibration

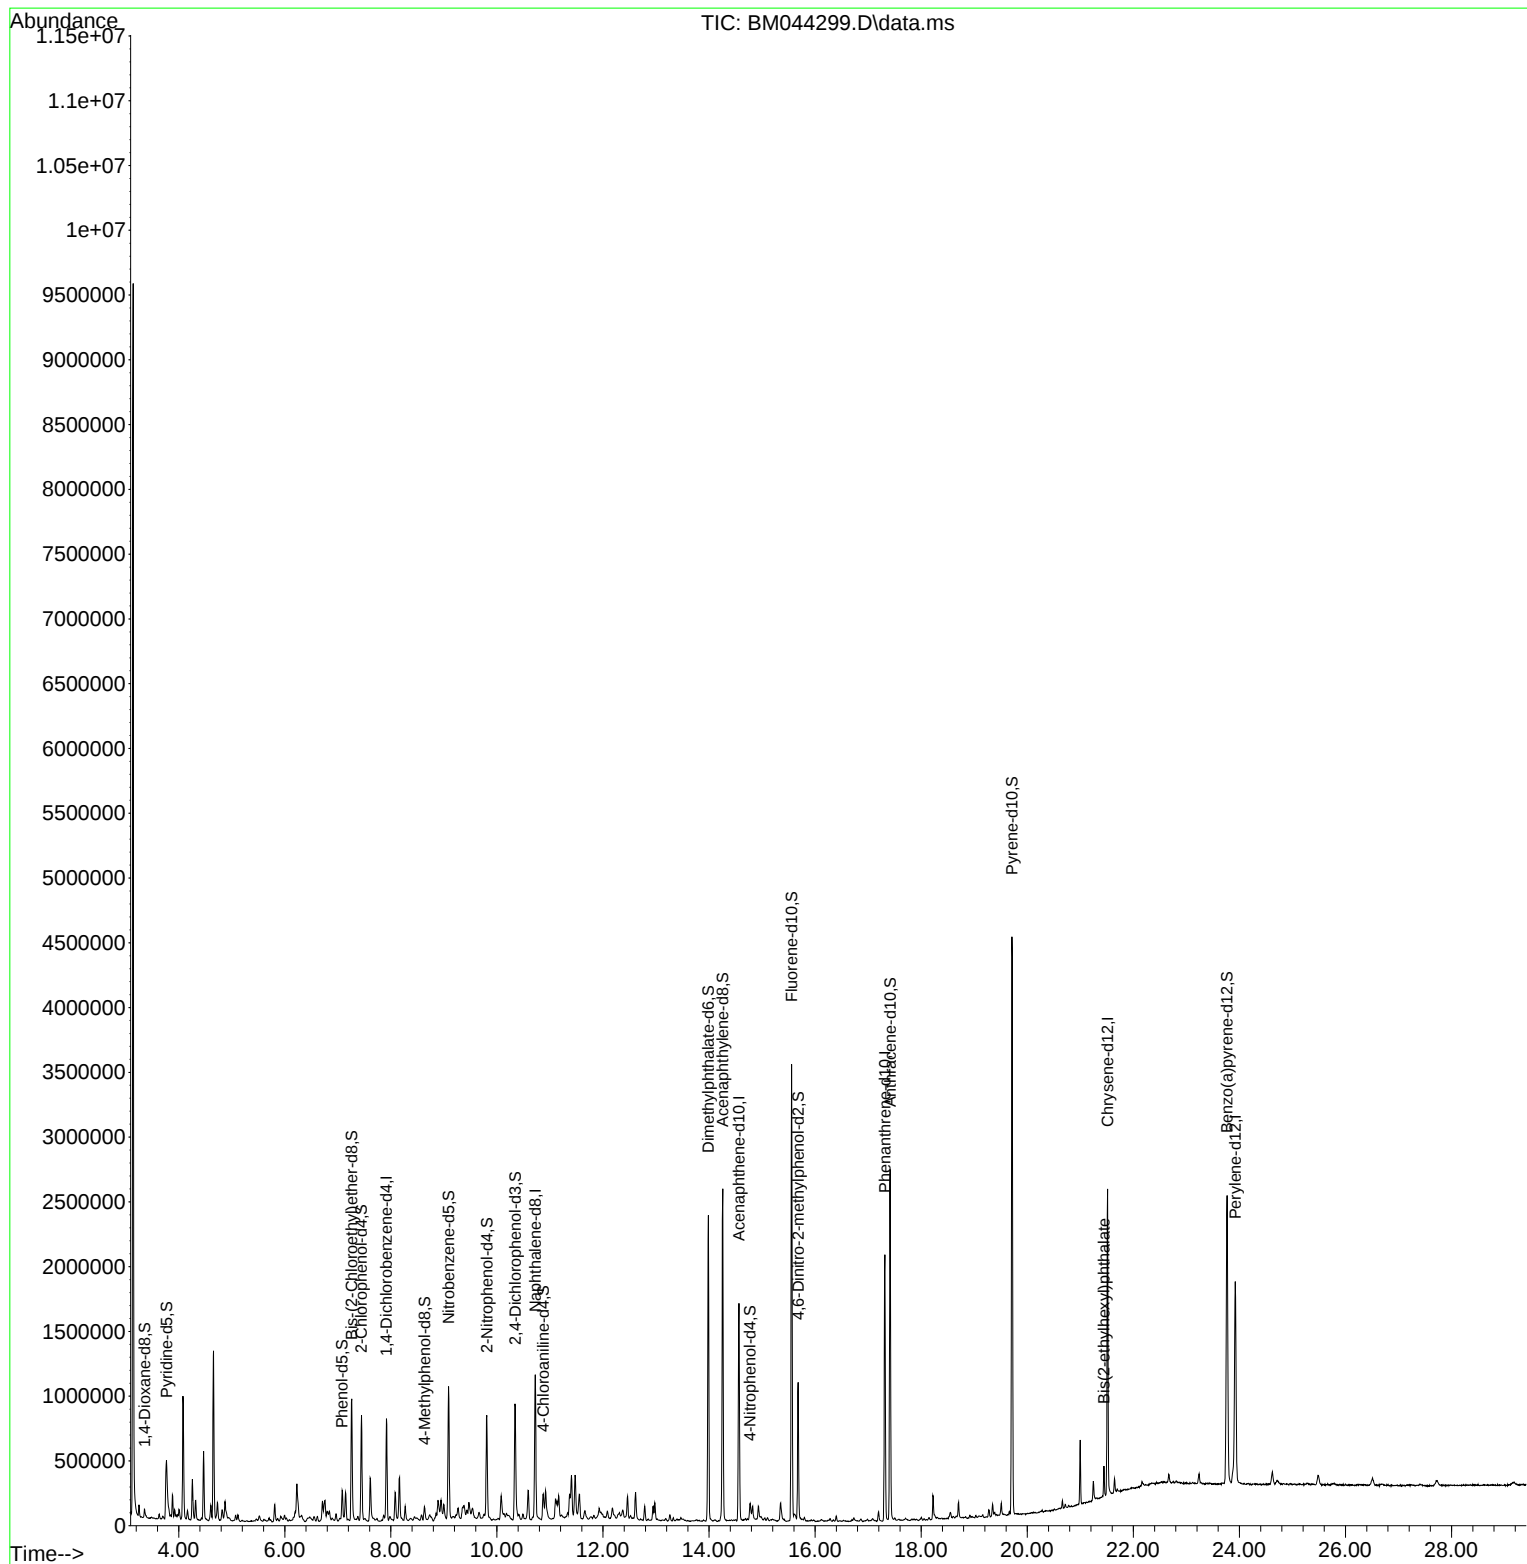

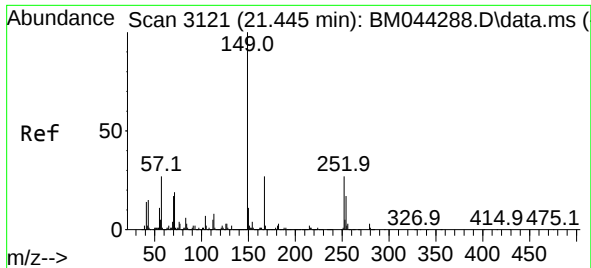

#86  
 Bis(2-ethylhexyl)phthalate  
 Concen: 1.335 ng/ul  
 RT: 21.445 min Scan# 31  
 Delta R.T. -0.000 min  
 Lab File: BM044299.D  
 Acq: 24 Feb 2024 17:29

Instrument :  
 BNA\_M  
 ClientSampleId :  
 C0AB6

|           |       |       |       |
|-----------|-------|-------|-------|
| Tgt Ion:  | 149   | Resp: | 75515 |
| Ion Ratio | Lower | Upper |       |
| 149       | 100   |       |       |
| 167       | 28.3  | 22.1  | 33.1  |
| 279       | 3.4   | 2.4   | 3.6   |

