

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
 Data File : BM044289.D
 Acq On : 24 Feb 2024 11:26
 Operator : MA/JU
 Sample : PB159154BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK154

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044289.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.357	42	46	53	rVB	104500	143720	2.39%	0.224%
2	3.769	112	116	136	rBV	1164787	1860871	30.94%	2.898%
3	4.093	168	171	174	rVB2	14710	18206	0.30%	0.028%
4	7.081	672	679	691	rBV	1224419	1922438	31.96%	2.994%
5	7.257	703	709	723	rVB	1048875	1686613	28.04%	2.626%
6	7.445	733	741	749	rBV	1213599	1953576	32.48%	3.042%
7	7.916	814	821	830	rVB	863793	1343036	22.33%	2.091%
8	8.628	935	942	957	rBV	1430600	2285533	38.00%	3.559%
9	9.086	1012	1020	1031	rBV	1107727	1817766	30.22%	2.831%
10	9.251	1045	1048	1054	rBV8	3805	6105	0.10%	0.010%
11	9.804	1133	1142	1153	rBV	880598	1455248	24.19%	2.266%
12	10.339	1225	1233	1252	rBV	1280445	2184909	36.32%	3.402%
13	10.722	1290	1298	1310	rVB	1122482	1893115	31.47%	2.948%
14	10.869	1315	1323	1338	rBV	1321390	2371492	39.43%	3.693%
15	12.316	1563	1569	1578	rVB2	21841	39434	0.66%	0.061%
16	13.463	1758	1764	1771	rBV4	15106	28677	0.48%	0.045%
17	13.986	1846	1853	1867	rBV	2155661	3110234	51.71%	4.843%
18	14.257	1891	1899	1909	rBV	2547351	3867595	64.30%	6.023%
19	14.562	1944	1951	1959	rBV	1558647	2303149	38.29%	3.587%
20	14.768	1979	1986	2016	rBV	672199	1540245	25.61%	2.399%
21	14.974	2019	2021	2026	rVB5	3750	7060	0.12%	0.011%
22	15.557	2113	2120	2132	rBV	3202915	4684895	77.88%	7.295%
23	15.674	2134	2140	2156	rVV	1033187	1517607	25.23%	2.363%
24	15.798	2156	2161	2167	rVB5	16742	28207	0.47%	0.044%
25	16.339	2249	2253	2260	rVB6	11000	17471	0.29%	0.027%
26	17.309	2412	2418	2429	rBV	1800633	2657657	44.18%	4.139%
27	17.409	2429	2435	2452	rVV	3375789	5002226	83.16%	7.790%
28	18.227	2569	2574	2579	rBV6	17521	32731	0.54%	0.051%
29	19.274	2748	2752	2758	rVB2	37914	53994	0.90%	0.084%
30	19.345	2759	2764	2769	rVB	35274	49474	0.82%	0.077%
31	19.509	2789	2792	2798	rBV6	12764	18104	0.30%	0.028%
32	19.709	2820	2826	2835	rVV	4278817	5763036	95.81%	8.974%
33	21.515	3127	3133	3146	rBV	2103230	2855315	47.47%	4.446%
34	23.233	3422	3425	3433	rVB	97169	150634	2.50%	0.235%
35	23.768	3508	3516	3529	rBV2	2916428	6015197	100.00%	9.367%
36	23.921	3531	3542	3552	rVB	1487148	3274595	54.44%	5.099%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044289.D
Acq On : 24 Feb 2024 11:26
Operator : MA/JU
Sample : PB159154BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK154

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37	24.621	3657	3661	3669	rVB2	132342	256382	4.26%	0.399%
----	--------	------	------	------	------	--------	--------	-------	--------




Sum of corrected areas: 64216547

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044289.D
Acq On : 24 Feb 2024 11:26
Operator : MA/JU
Sample : PB159154BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK154

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

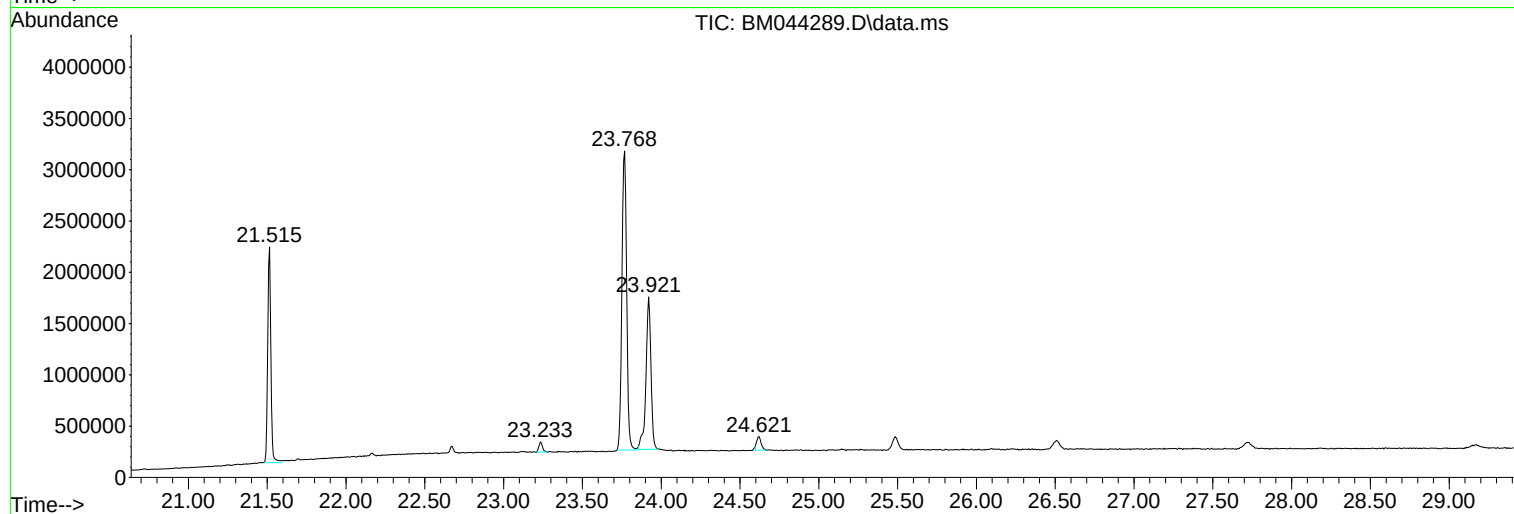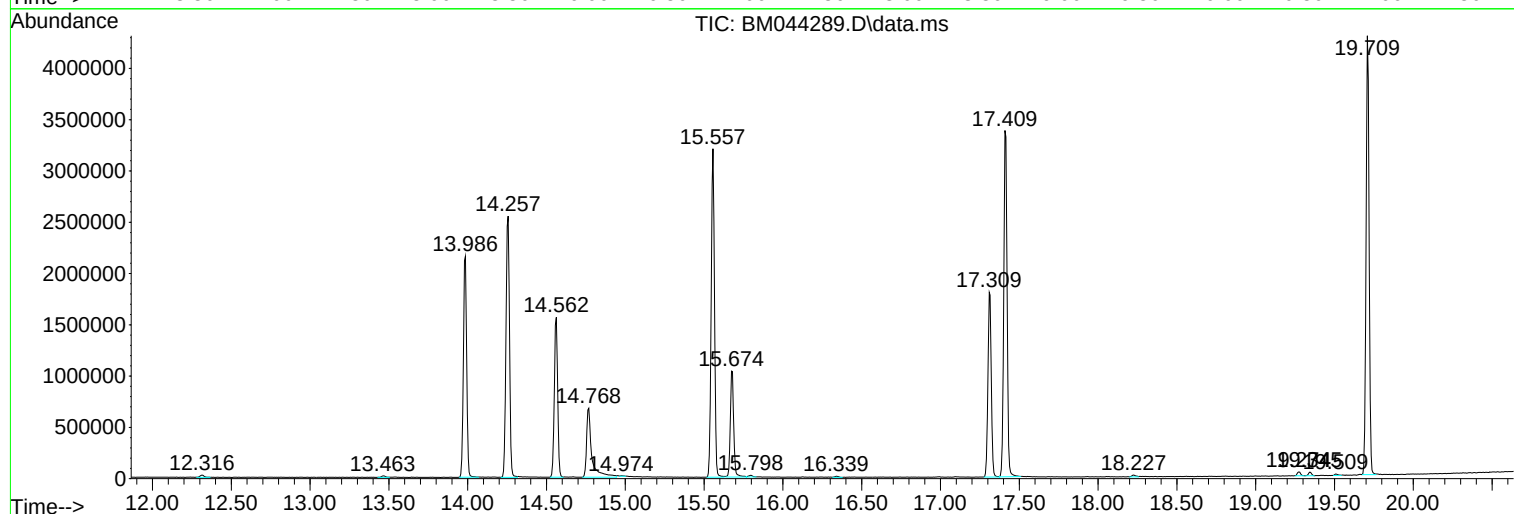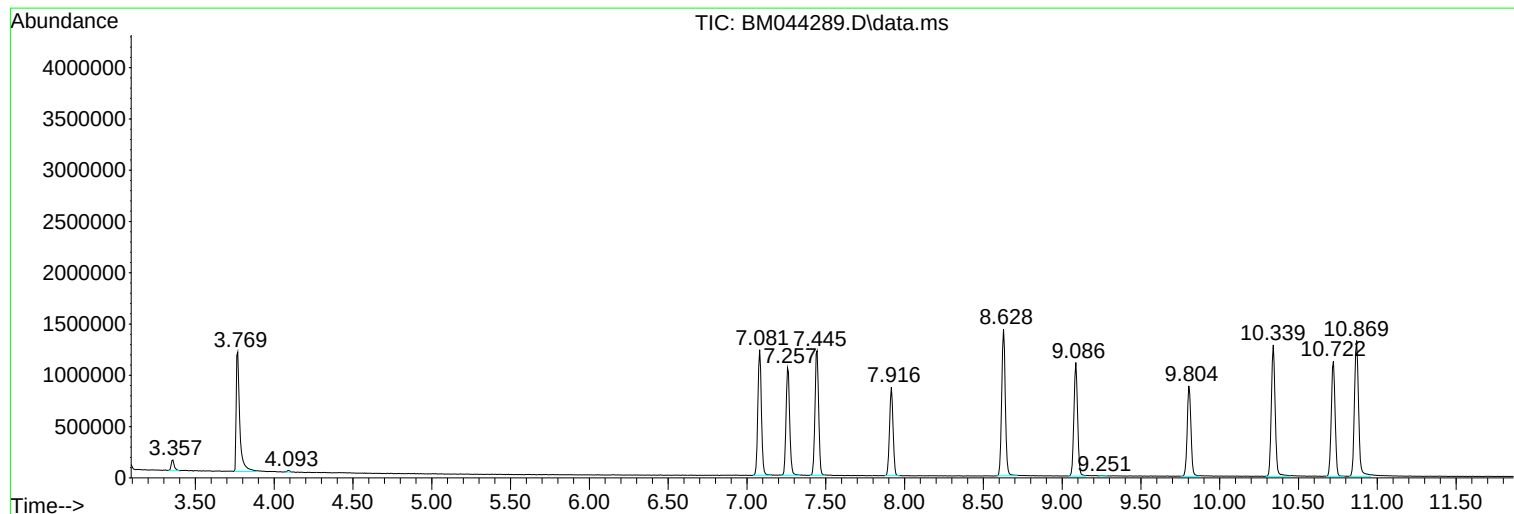

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044289.D
Acq On : 24 Feb 2024 11:26
Operator : MA/JU
Sample : PB159154BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK154

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044289.D
Acq On : 24 Feb 2024 11:26
Operator : MA/JU
Sample : PB159154BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK154

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------