

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
 Data File : BM044290.D
 Acq On : 24 Feb 2024 12:02
 Operator : MA/JU
 Sample : PB159156BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK156

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044290.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	42	45	53	rBV	102867	136865	2.17%	0.196%
2	3.763	112	115	143	rBV	1192675	1924336	30.50%	2.749%
3	4.093	168	171	175	rVB	19811	23308	0.37%	0.033%
4	7.081	672	679	689	rBV	1267012	1960817	31.07%	2.801%
5	7.257	703	709	721	rVB	1073055	1699757	26.94%	2.428%
6	7.445	733	741	752	rBV	1251270	1982727	31.42%	2.833%
7	7.916	814	821	830	rBV	1062419	1647026	26.10%	2.353%
8	8.628	935	942	952	rBV	1468616	2341891	37.11%	3.346%
9	9.087	1012	1020	1037	rBV	1126483	1862645	29.52%	2.661%
10	9.804	1135	1142	1157	rBV	885235	1486075	23.55%	2.123%
11	10.339	1226	1233	1246	rBV	1331926	2234889	35.42%	3.193%
12	10.722	1289	1298	1305	rBV	1389960	2343615	37.14%	3.348%
13	10.869	1315	1323	1340	rBV	1366548	2465481	39.07%	3.523%
14	12.316	1562	1569	1575	rBV2	21881	39600	0.63%	0.057%
15	13.463	1759	1764	1769	rBV2	19401	31334	0.50%	0.045%
16	13.527	1772	1775	1782	rVB8	4098	7557	0.12%	0.011%
17	13.980	1846	1852	1863	rBV	2303669	3319397	52.60%	4.743%
18	14.257	1891	1899	1911	rBV	2691272	4052455	64.22%	5.790%
19	14.563	1944	1951	1960	rBV	1975967	2953600	46.81%	4.220%
20	14.763	1979	1985	2020	rBV	754318	1677479	26.58%	2.397%
21	15.557	2113	2120	2133	rBV	3433959	4979088	78.91%	7.114%
22	15.674	2134	2140	2155	rVV	1143010	1640895	26.00%	2.344%
23	15.798	2157	2161	2165	rVB3	12912	21418	0.34%	0.031%
24	16.345	2250	2254	2258	rVB5	11759	18199	0.29%	0.026%
25	16.992	2360	2364	2368	rVB5	5225	6753	0.11%	0.010%
26	17.098	2379	2382	2387	rVB3	5148	6324	0.10%	0.009%
27	17.310	2412	2418	2429	rBV	2377450	3467833	54.96%	4.955%
28	17.410	2429	2435	2452	rVB2	3600445	5358936	84.93%	7.656%
29	18.227	2568	2574	2581	rBV8	18814	35904	0.57%	0.051%
30	19.274	2747	2752	2758	rVB3	45363	60135	0.95%	0.086%
31	19.345	2758	2764	2771	rBV	41459	60900	0.97%	0.087%
32	19.509	2788	2792	2797	rBV6	14605	23624	0.37%	0.034%
33	19.662	2815	2818	2820	rBV3	13076	14566	0.23%	0.021%
34	19.709	2820	2826	2836	rVV	4631699	6131497	97.17%	8.760%
35	21.509	3127	3132	3144	rBV	2755402	3641027	57.70%	5.202%
36	23.762	3507	3515	3528	rBV2	3238816	6310123	100.00%	9.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044290.D
Acq On : 24 Feb 2024 12:02
Operator : MA/JU
Sample : PB159156BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK156

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37 23.921 3535 3542 3560 rVB 1875000 4024058 63.77% 5.749%




Sum of corrected areas: 69992134

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044290.D
Acq On : 24 Feb 2024 12:02
Operator : MA/JU
Sample : PB159156BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK156

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

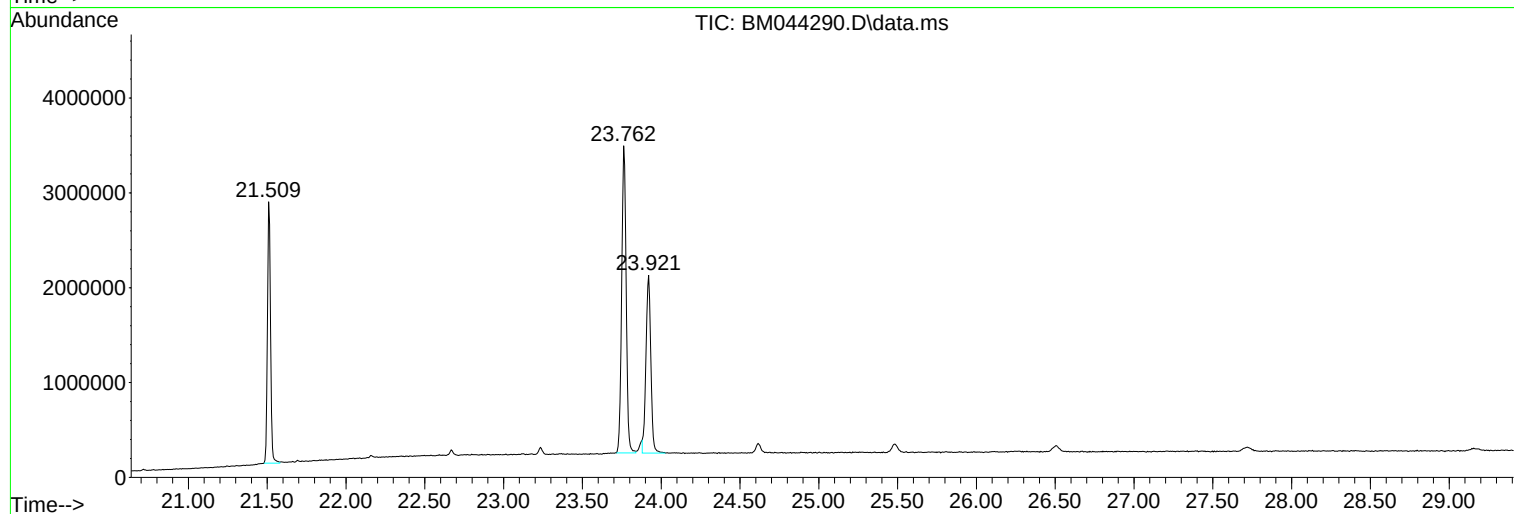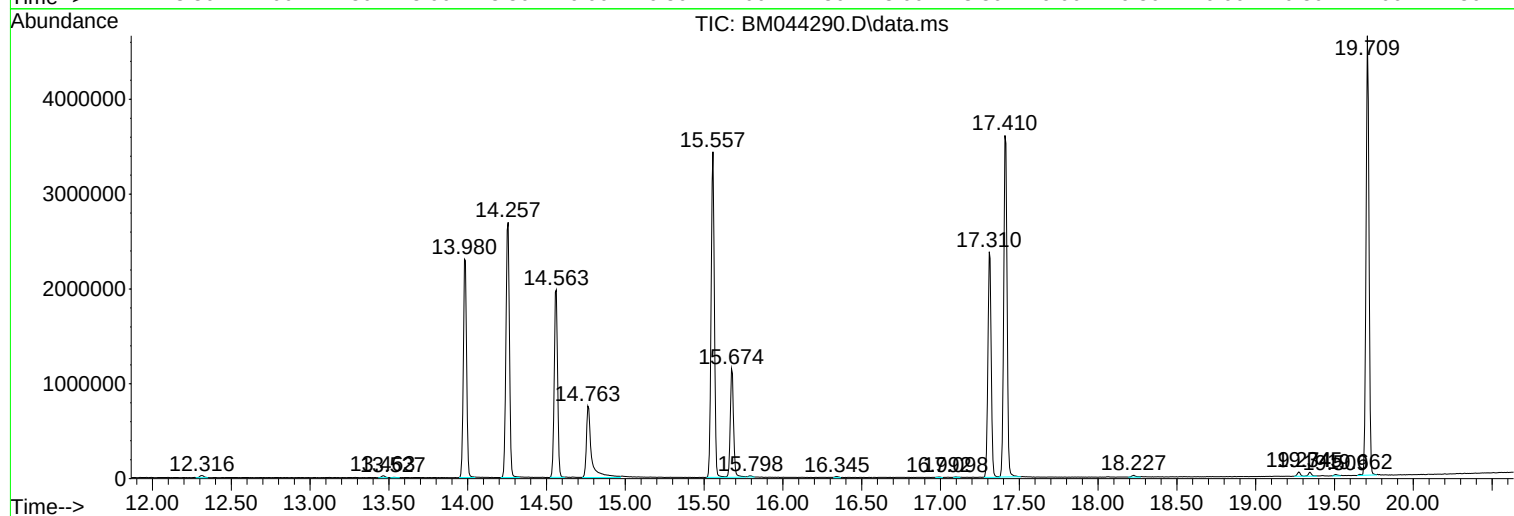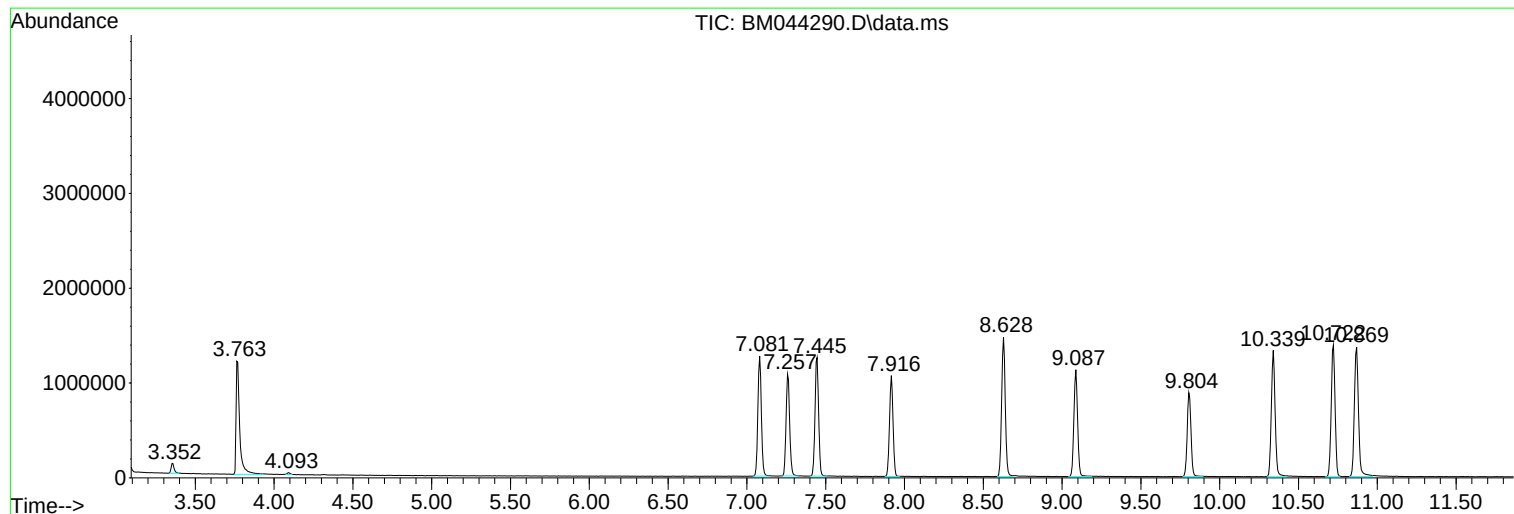

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044290.D
Acq On : 24 Feb 2024 12:02
Operator : MA/JU
Sample : PB159156BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK156

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044290.D
Acq On : 24 Feb 2024 12:02
Operator : MA/JU
Sample : PB159156BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK156

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------