

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
 Data File : BM044306.D
 Acq On : 24 Feb 2024 22:21
 Operator : MA/JU
 Sample : PB159148BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK148

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044306.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.357	42	46	56	rVB	90862	113715	2.07%	0.193%
2	3.769	113	116	139	rBV	1001820	1557131	28.30%	2.646%
3	4.093	168	171	175	rVB	14808	18790	0.34%	0.032%
4	7.087	673	680	693	rBV	998614	1553352	28.23%	2.640%
5	7.263	704	710	722	rBV	852388	1336889	24.30%	2.272%
6	7.451	734	742	751	rBV	964827	1562866	28.41%	2.656%
7	7.922	815	822	831	rVB	856310	1336742	24.30%	2.272%
8	8.633	935	943	961	rBV	1166882	1907423	34.67%	3.242%
9	9.092	1011	1021	1029	rBV	895682	1478125	26.87%	2.512%
10	9.257	1043	1049	1056	rVB10	6261	14506	0.26%	0.025%
11	9.810	1137	1143	1156	rBV	715553	1190320	21.64%	2.023%
12	10.345	1226	1234	1255	rBV	1051073	1819955	33.08%	3.093%
13	10.727	1291	1299	1309	rVB	1168762	1934769	35.17%	3.288%
14	10.875	1316	1324	1338	rBV	1097962	1992784	36.22%	3.387%
15	12.321	1564	1570	1575	rBV2	18350	32822	0.60%	0.056%
16	13.474	1760	1766	1769	rBV	19378	30915	0.56%	0.053%
17	13.986	1847	1853	1867	rBV	1959478	2762184	50.21%	4.694%
18	14.257	1892	1899	1912	rBV	2177306	3355479	60.99%	5.702%
19	14.563	1945	1951	1959	rBV	1650670	2511149	45.64%	4.268%
20	14.774	1980	1987	2004	rBV	583147	1299254	23.62%	2.208%
21	15.562	2113	2121	2134	rBV	2789495	4183880	76.05%	7.110%
22	15.680	2135	2141	2157	rVV	952477	1331892	24.21%	2.263%
23	15.798	2158	2161	2167	rVB5	14886	21598	0.39%	0.037%
24	16.345	2251	2254	2259	rVB4	8776	11283	0.21%	0.019%
25	16.992	2359	2364	2369	rBV8	5462	10182	0.19%	0.017%
26	17.315	2413	2419	2429	rBV	2156515	3029926	55.07%	5.149%
27	17.415	2429	2436	2450	rVV	3192432	4584573	83.33%	7.791%
28	18.233	2568	2575	2581	rBV7	17488	35785	0.65%	0.061%
29	19.280	2748	2753	2757	rBV2	38609	52408	0.95%	0.089%
30	19.350	2760	2765	2770	rBV	33654	49694	0.90%	0.084%
31	19.509	2789	2792	2798	rBV7	15767	19667	0.36%	0.033%
32	19.715	2821	2827	2836	rBV	4066425	5362002	97.46%	9.112%
33	21.515	3127	3133	3144	rBV	2544271	3328165	60.49%	5.656%
34	23.768	3508	3516	3529	rBV2	2713299	5501561	100.00%	9.350%
35	23.921	3536	3542	3555	rVB	1658855	3511504	63.83%	5.968%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044306.D
Acq On : 24 Feb 2024 22:21
Operator : MA/JU
Sample : PB159148BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK148

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 58843290

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044306.D
Acq On : 24 Feb 2024 22:21
Operator : MA/JU
Sample : PB159148BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK148

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

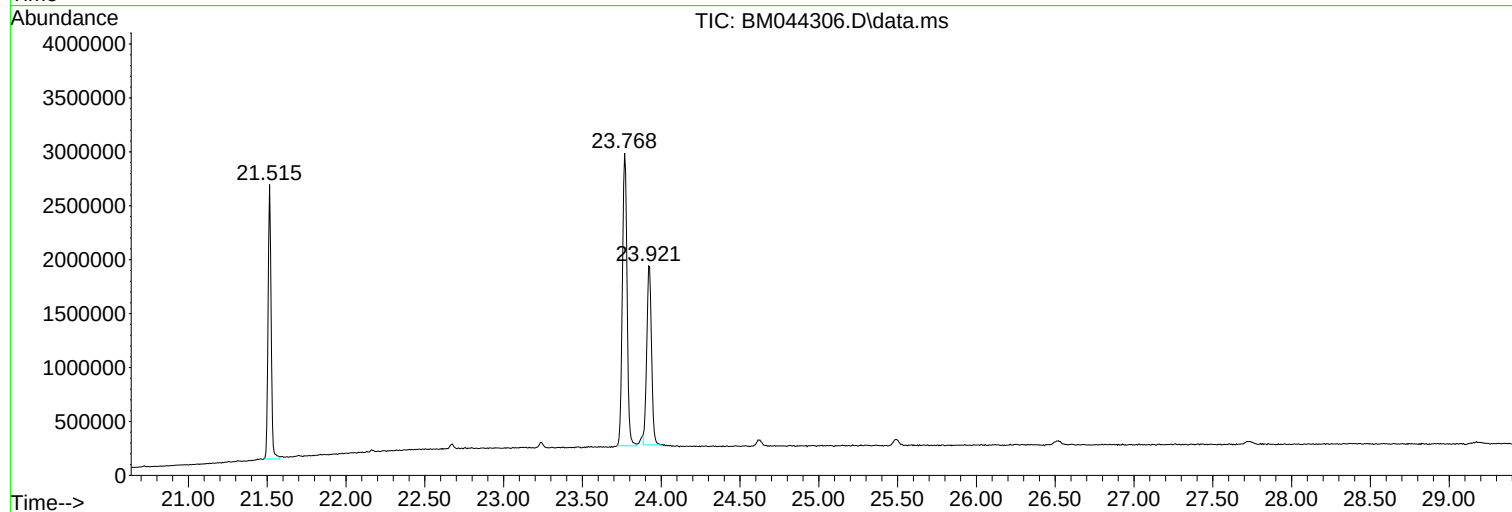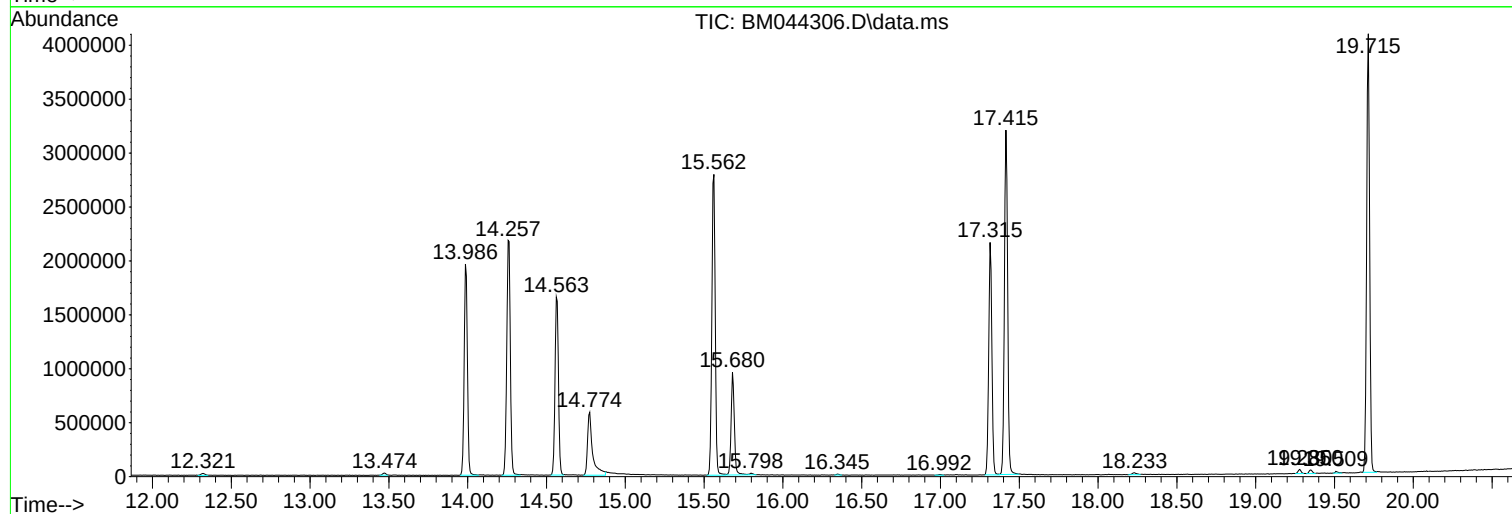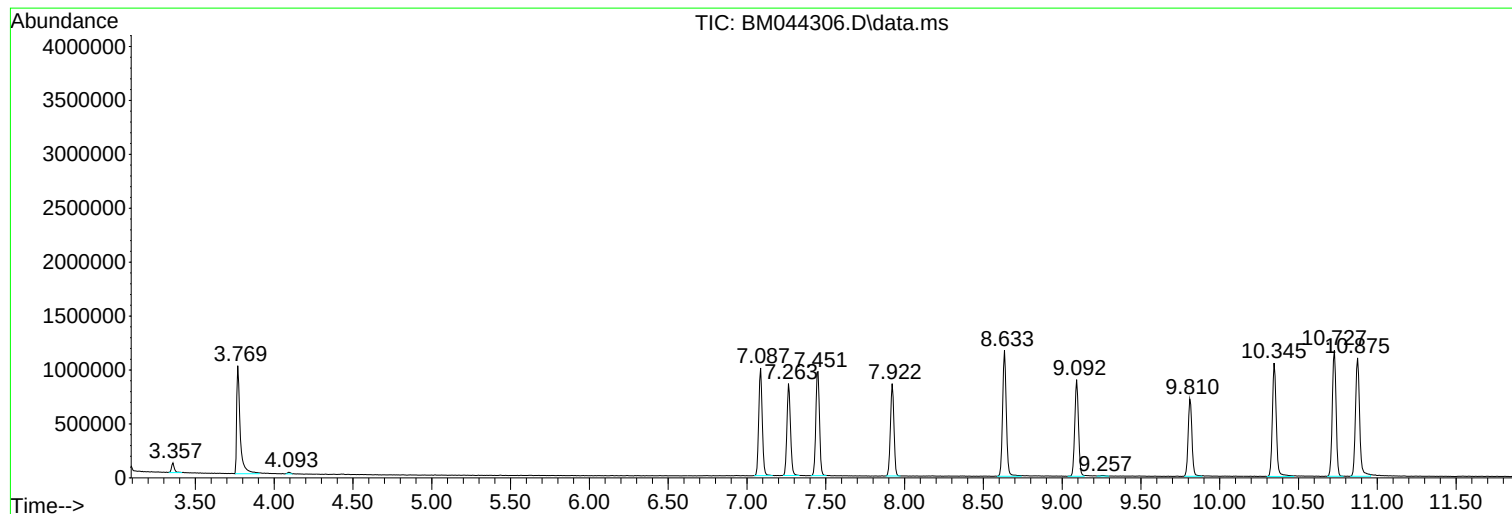

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044306.D
Acq On : 24 Feb 2024 22:21
Operator : MA/JU
Sample : PB159148BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK148

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044306.D
Acq On : 24 Feb 2024 22:21
Operator : MA/JU
Sample : PB159148BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK148

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------