

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
 Data File : BM044307.D
 Acq On : 24 Feb 2024 22:57
 Operator : MA/JU
 Sample : PB159150BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK150

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044307.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.357	42	46	52	rVB	87980	108647	1.96%	0.181%
2	3.769	112	116	138	rBV	1085672	1661279	30.03%	2.770%
3	4.093	168	171	180	rVB	16792	27616	0.50%	0.046%
4	7.087	673	680	690	rBV	1075782	1669750	30.18%	2.784%
5	7.263	704	710	725	rBV	896610	1435583	25.95%	2.393%
6	7.451	734	742	755	rBV	1044236	1673841	30.26%	2.791%
7	7.922	815	822	829	rVB	811522	1268794	22.94%	2.115%
8	8.634	936	943	961	rBV	1262281	2022453	36.56%	3.372%
9	9.092	1013	1021	1035	rBV	961259	1590071	28.74%	2.651%
10	9.257	1045	1049	1054	rBV6	4747	7048	0.13%	0.012%
11	9.810	1136	1143	1157	rBV	749177	1267908	22.92%	2.114%
12	10.345	1226	1234	1247	rBV	1153354	1946691	35.19%	3.246%
13	10.728	1291	1299	1308	rBV	1114844	1866787	33.75%	3.112%
14	10.875	1315	1324	1348	rBV	1193141	2181156	39.43%	3.637%
15	12.322	1564	1570	1577	rVB	20168	34654	0.63%	0.058%
16	13.469	1758	1765	1770	rBV2	22787	35776	0.65%	0.060%
17	13.992	1847	1854	1868	rBV	2028177	2937294	53.10%	4.897%
18	14.257	1891	1899	1913	rBV	2390135	3604874	65.16%	6.010%
19	14.569	1945	1952	1960	rBV	1635603	2420115	43.75%	4.035%
20	14.774	1979	1987	2012	rBV	629510	1419863	25.67%	2.367%
21	15.563	2114	2121	2134	rBV	3088465	4444959	80.35%	7.411%
22	15.680	2134	2141	2152	rVV	955852	1348180	24.37%	2.248%
23	15.804	2157	2162	2168	rVB3	15132	27191	0.49%	0.045%
24	16.127	2214	2217	2223	rBV6	3953	5703	0.10%	0.010%
25	16.345	2247	2254	2259	rBV7	8945	17217	0.31%	0.029%
26	17.315	2412	2419	2430	rBV	1998690	2879615	52.05%	4.801%
27	17.415	2430	2436	2448	rVV2	3356403	4819443	87.12%	8.035%
28	18.227	2570	2574	2580	rBV7	16333	24265	0.44%	0.040%
29	19.280	2749	2753	2759	rBV2	41133	53813	0.97%	0.090%
30	19.351	2760	2765	2769	rBV2	34257	48385	0.87%	0.081%
31	19.509	2789	2792	2799	rBV6	9969	15717	0.28%	0.026%
32	19.668	2817	2819	2821	rBV2	6425	5597	0.10%	0.009%
33	19.715	2821	2827	2836	rVV	4168726	5532002	100.00%	9.223%
34	21.515	3128	3133	3144	rBV	2228902	2971901	53.72%	4.955%
35	23.768	3509	3516	3530	rVB2	2658685	5424146	98.05%	9.043%
36	23.927	3536	3543	3559	rVB	1499574	3180805	57.50%	5.303%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044307.D
Acq On : 24 Feb 2024 22:57
Operator : MA/JU
Sample : PB159150BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK150

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 59979139

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044307.D
Acq On : 24 Feb 2024 22:57
Operator : MA/JU
Sample : PB159150BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK150

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

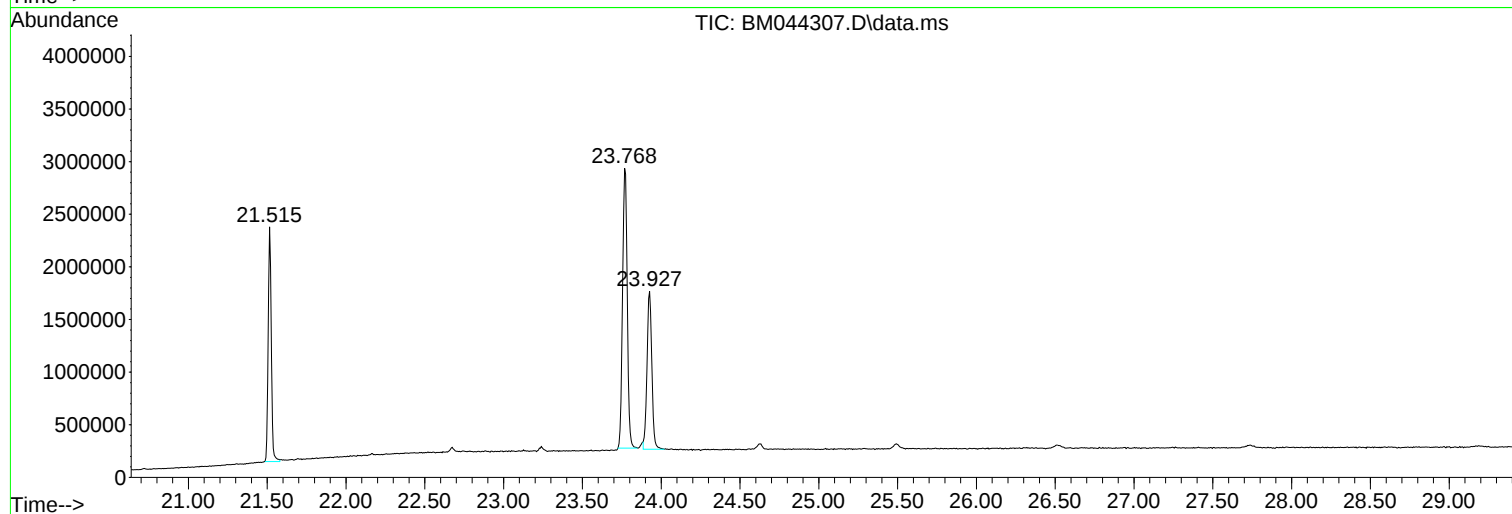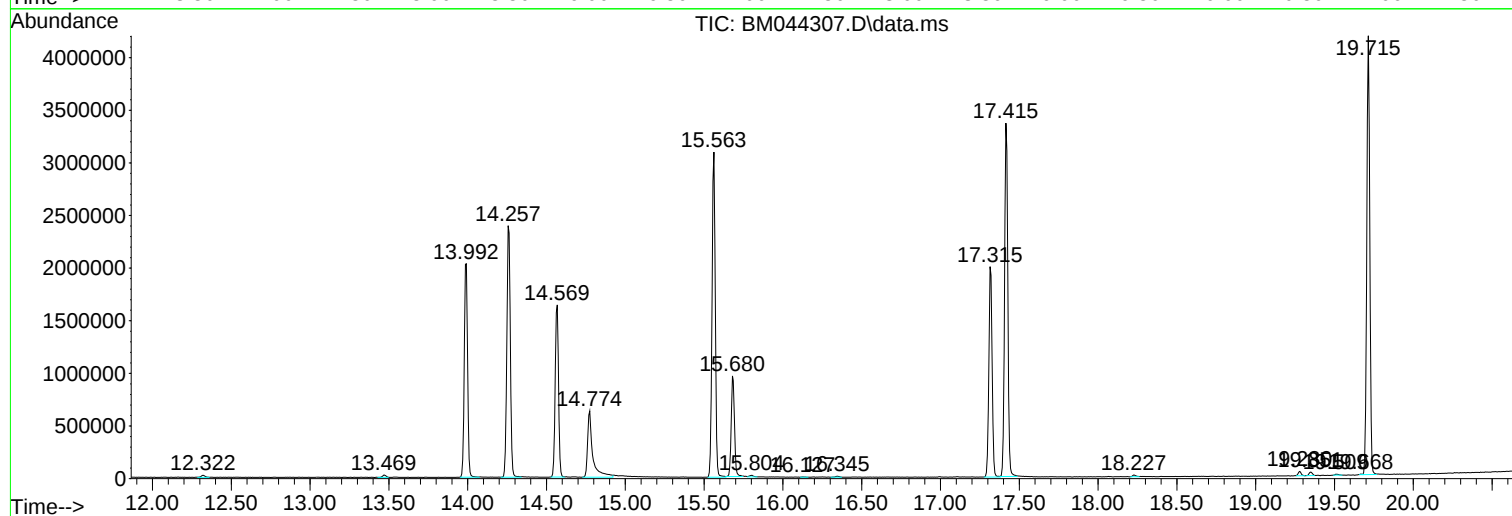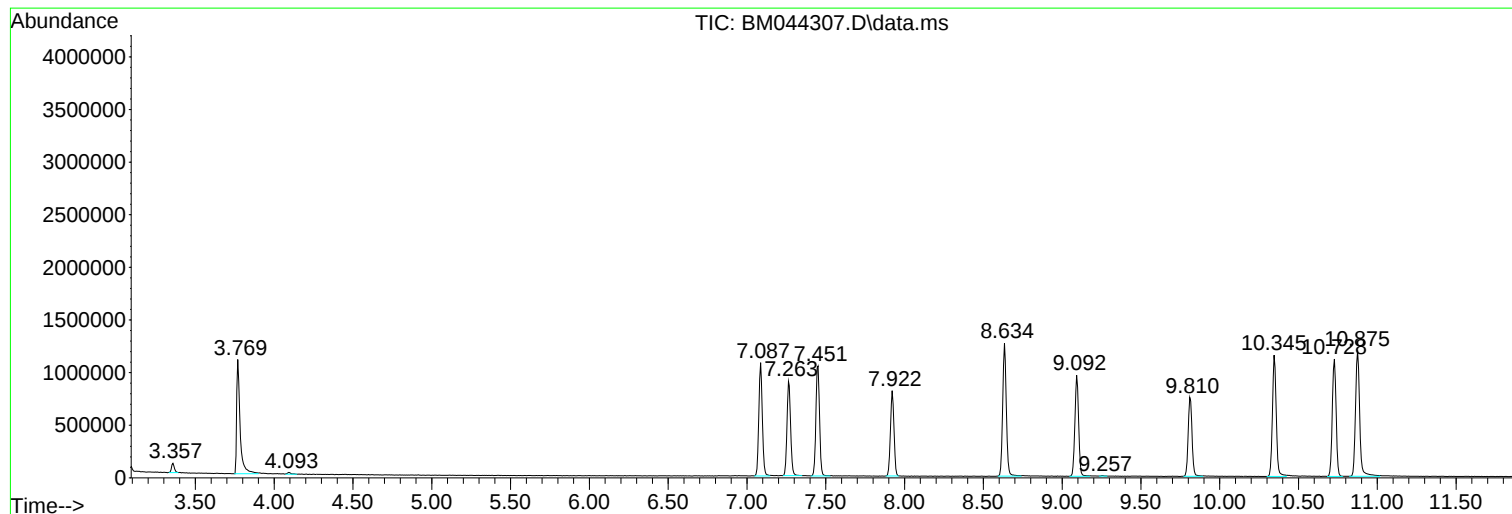

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044307.D
Acq On : 24 Feb 2024 22:57
Operator : MA/JU
Sample : PB159150BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK150

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044307.D
Acq On : 24 Feb 2024 22:57
Operator : MA/JU
Sample : PB159150BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK150

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------