

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
 Data File : BM044308.D
 Acq On : 24 Feb 2024 23:33
 Operator : MA/JU
 Sample : PB159152BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK152

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044308.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.357	42	46	54	rVB	92298	114870	2.05%	0.202%
2	3.769	112	116	143	rBV	1038450	1617980	28.94%	2.845%
3	4.093	168	171	179	rVB2	16340	23897	0.43%	0.042%
4	7.087	673	680	690	rBV	1013222	1609710	28.79%	2.831%
5	7.263	704	710	721	rBV	847623	1374250	24.58%	2.417%
6	7.451	734	742	752	rBV	1015540	1602846	28.67%	2.819%
7	7.922	815	822	831	rVB	701208	1105790	19.78%	1.945%
8	8.634	936	943	952	rBV	1187256	1909660	34.16%	3.358%
9	9.092	1012	1021	1031	rBV	917206	1510466	27.02%	2.656%
10	9.810	1136	1143	1159	rBV	696486	1206646	21.58%	2.122%
11	10.345	1226	1234	1253	rBV	1067142	1848984	33.07%	3.252%
12	10.728	1289	1299	1309	rBV	953134	1596348	28.55%	2.807%
13	10.875	1315	1324	1341	rBV	1115560	2045822	36.59%	3.598%
14	12.322	1562	1570	1576	rVB2	17815	31094	0.56%	0.055%
15	13.474	1759	1766	1773	rBV4	19354	35286	0.63%	0.062%
16	13.551	1775	1779	1783	rVB6	3862	6555	0.12%	0.012%
17	13.992	1847	1854	1870	rBV	1958046	2813106	50.32%	4.947%
18	14.263	1892	1900	1913	rBV	2253935	3408221	60.96%	5.994%
19	14.568	1944	1952	1961	rBV	1350315	2061106	36.87%	3.625%
20	14.774	1980	1987	2012	rBV	597474	1371085	24.52%	2.411%
21	15.563	2114	2121	2135	rBV	2892638	4248813	76.00%	7.472%
22	15.680	2135	2141	2158	rVV	931170	1356461	24.26%	2.386%
23	15.798	2158	2161	2166	rVB2	13221	21818	0.39%	0.038%
24	16.351	2250	2255	2259	rVB6	8896	13847	0.25%	0.024%
25	16.998	2360	2365	2370	rVB8	5260	6334	0.11%	0.011%
26	17.104	2379	2383	2387	rBV6	3657	6856	0.12%	0.012%
27	17.315	2413	2419	2429	rBV	1719229	2508301	44.86%	4.411%
28	17.415	2429	2436	2448	rVV	3281595	4672385	83.57%	8.217%
29	18.227	2571	2574	2579	rBV6	12586	19775	0.35%	0.035%
30	19.280	2749	2753	2757	rVV2	40979	55606	0.99%	0.098%
31	19.351	2760	2765	2772	rBV	35628	54439	0.97%	0.096%
32	19.515	2790	2793	2798	rBV6	12769	15324	0.27%	0.027%
33	19.668	2816	2819	2821	rBV3	6548	6880	0.12%	0.012%
34	19.715	2821	2827	2839	rVV	4075436	5464965	97.75%	9.611%
35	21.515	3128	3133	3146	rBV	1953945	2698223	48.26%	4.745%
36	23.774	3509	3517	3531	rBV2	2786990	5590876	100.00%	9.832%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044308.D
Acq On : 24 Feb 2024 23:33
Operator : MA/JU
Sample : PB159152BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK152

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37	23.927	3537	3543	3555	rVB	1371407	2827693	50.58%	4.973%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 56862318

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044308.D
Acq On : 24 Feb 2024 23:33
Operator : MA/JU
Sample : PB159152BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK152

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

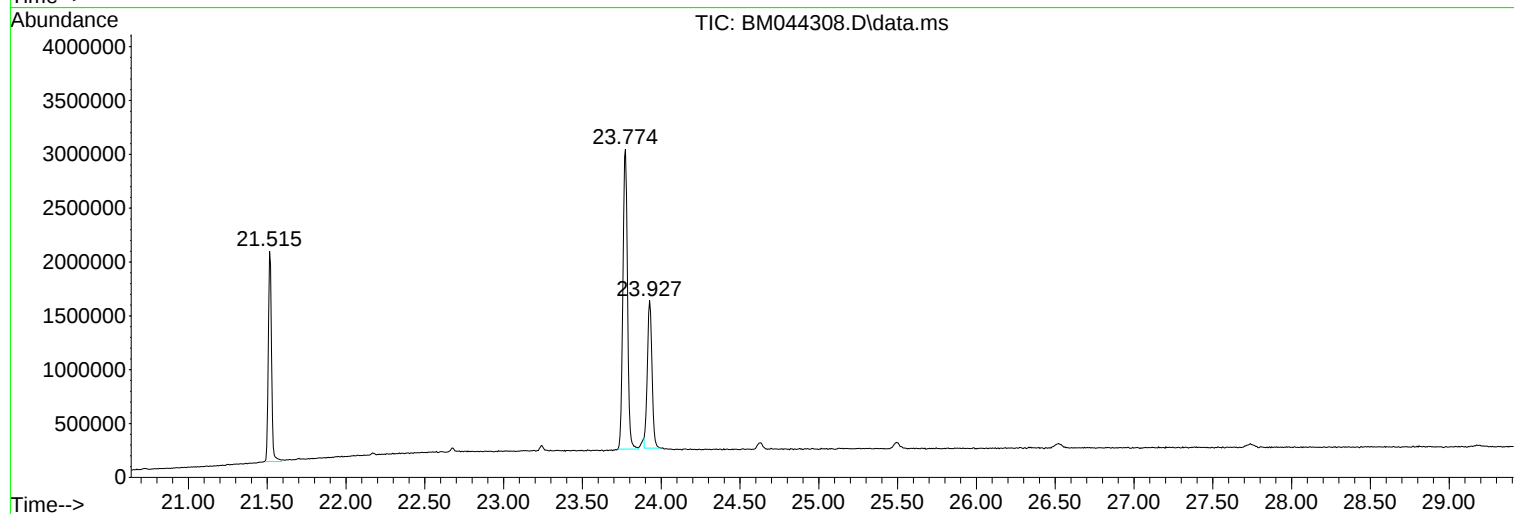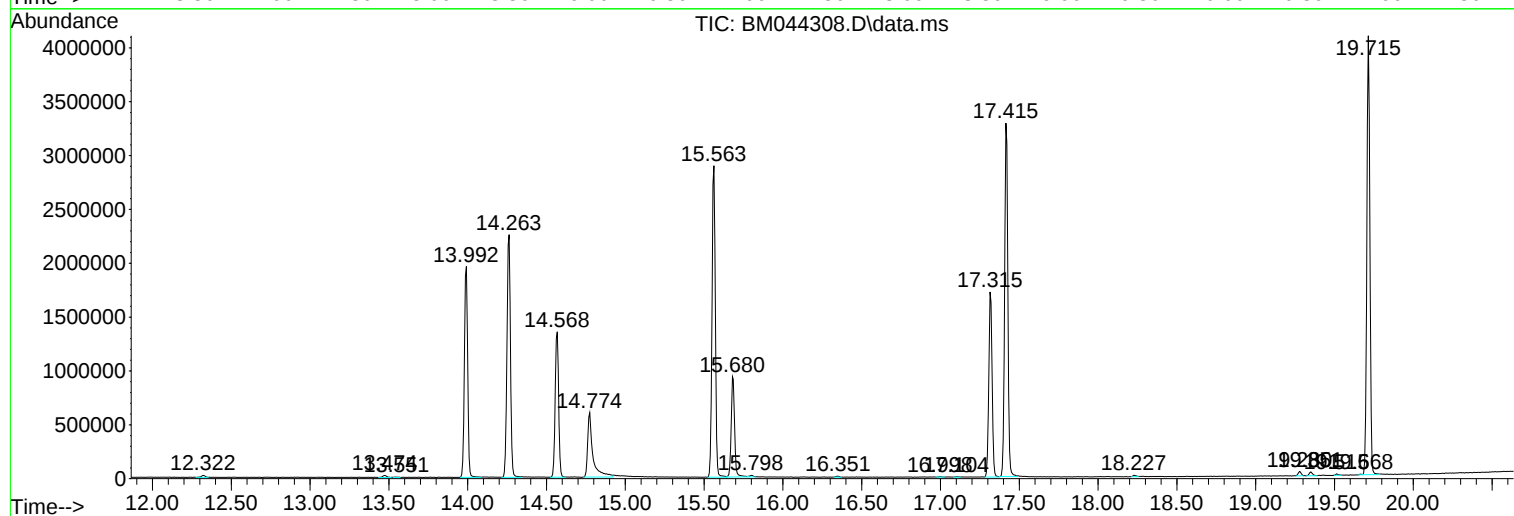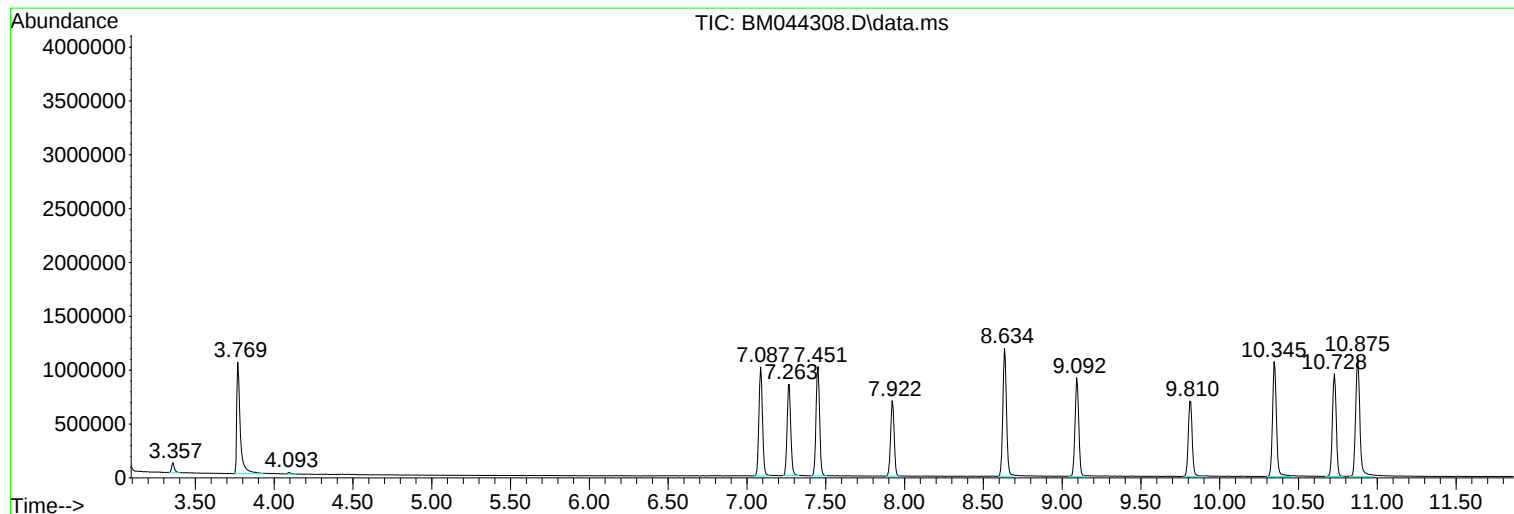

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044308.D
Acq On : 24 Feb 2024 23:33
Operator : MA/JU
Sample : PB159152BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK152

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044308.D
Acq On : 24 Feb 2024 23:33
Operator : MA/JU
Sample : PB159152BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK152

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------