

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
 Data File : BM044317.D
 Acq On : 25 Feb 2024 04:59
 Operator : MA/JU
 Sample : P1494-08
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH410

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044317.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.357	42	46	51	rBV	70293	87016	1.05%	0.119%
2	3.775	114	117	140	rBV	380627	653613	7.92%	0.895%
3	4.093	168	171	177	rVB	21374	30802	0.37%	0.042%
4	7.087	673	680	688	rBV	321749	507243	6.14%	0.694%
5	7.263	704	710	725	rVB	1163326	1833292	22.20%	2.510%
6	7.445	734	741	752	rBV	1060557	1723266	20.87%	2.359%
7	7.534	754	756	764	rVB7	6621	9836	0.12%	0.013%
8	7.922	815	822	831	rVB	889508	1393892	16.88%	1.908%
9	8.634	936	943	954	rBV	861130	1386028	16.79%	1.897%
10	9.092	1013	1021	1033	rBV	1249814	2073467	25.11%	2.838%
11	9.257	1046	1049	1053	rVB4	5341	8500	0.10%	0.012%
12	9.810	1135	1143	1157	rBV	988831	1657101	20.07%	2.268%
13	10.345	1226	1234	1249	rBV	1393005	2346779	28.42%	3.212%
14	10.728	1291	1299	1307	rBV	1217702	2068980	25.06%	2.832%
15	10.875	1316	1324	1333	rBV	1316562	2366919	28.67%	3.240%
16	11.398	1407	1413	1418	rBV7	3872	8763	0.11%	0.012%
17	11.545	1432	1438	1440	rBV7	5213	8845	0.11%	0.012%
18	12.316	1564	1569	1576	rBV	27728	47713	0.58%	0.065%
19	13.469	1759	1765	1772	rBV	24168	39235	0.48%	0.054%
20	13.986	1844	1853	1863	rBV	2756029	3969483	48.07%	5.434%
21	14.257	1892	1899	1912	rBV	3241485	4906882	59.43%	6.717%
22	14.563	1944	1951	1963	rBV	1830672	2747424	33.27%	3.761%
23	14.774	1981	1987	2007	rBV	112414	356587	4.32%	0.488%
24	14.992	2019	2024	2035	rVB	10106	27953	0.34%	0.038%
25	15.563	2114	2121	2135	rBV	4018996	6072662	73.55%	8.313%
26	15.680	2135	2141	2154	rVV	1530468	2173964	26.33%	2.976%
27	15.798	2158	2161	2172	rVB4	21474	40949	0.50%	0.056%
28	16.292	2241	2245	2250	rVB7	6504	11835	0.14%	0.016%
29	16.345	2250	2254	2260	rBV6	14105	22593	0.27%	0.031%
30	16.998	2361	2365	2368	rVB5	7217	8927	0.11%	0.012%
31	17.086	2376	2380	2384	rBV4	11168	18217	0.22%	0.025%
32	17.315	2412	2419	2429	rBV	2285944	3266219	39.56%	4.471%
33	17.415	2429	2436	2452	rVV2	4848020	7028607	85.12%	9.621%
34	17.833	2502	2507	2510	rBV4	10697	14736	0.18%	0.020%
35	18.227	2569	2574	2580	rBV	88962	132024	1.60%	0.181%
36	18.527	2621	2625	2627	rBV4	12258	15159	0.18%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044317.D
Acq On : 25 Feb 2024 04:59
Operator : MA/JU
Sample : P1494-08
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH410

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37	18.715	2653	2657	2660	rVB6	5590	8508	0.10%	0.012%
38	19.168	2730	2734	2737	rBV5	8202	13569	0.16%	0.019%
39	19.280	2748	2753	2757	rBV	60382	83397	1.01%	0.114%
40	19.345	2760	2764	2769	rBV	53181	77980	0.94%	0.107%
41	19.421	2775	2777	2781	rVB4	10553	12206	0.15%	0.017%
42	19.509	2787	2792	2798	rBV2	69257	99534	1.21%	0.136%
43	19.662	2814	2818	2821	rBV2	28612	37034	0.45%	0.051%
44	19.715	2821	2827	2837	rVV	6070214	8198054	99.29%	11.222%
45	20.721	2995	2998	3001	rVB3	23550	23069	0.28%	0.032%
46	21.515	3127	3133	3145	rBV	2658864	3497555	42.36%	4.788%
47	23.768	3508	3516	3528	rBV2	4129978	8256945	100.00%	11.303%
48	23.921	3536	3542	3559	rVB	1761771	3679242	44.56%	5.036%




Sum of corrected areas: 73052604

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044317.D
Acq On : 25 Feb 2024 04:59
Operator : MA/JU
Sample : P1494-08
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH410

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

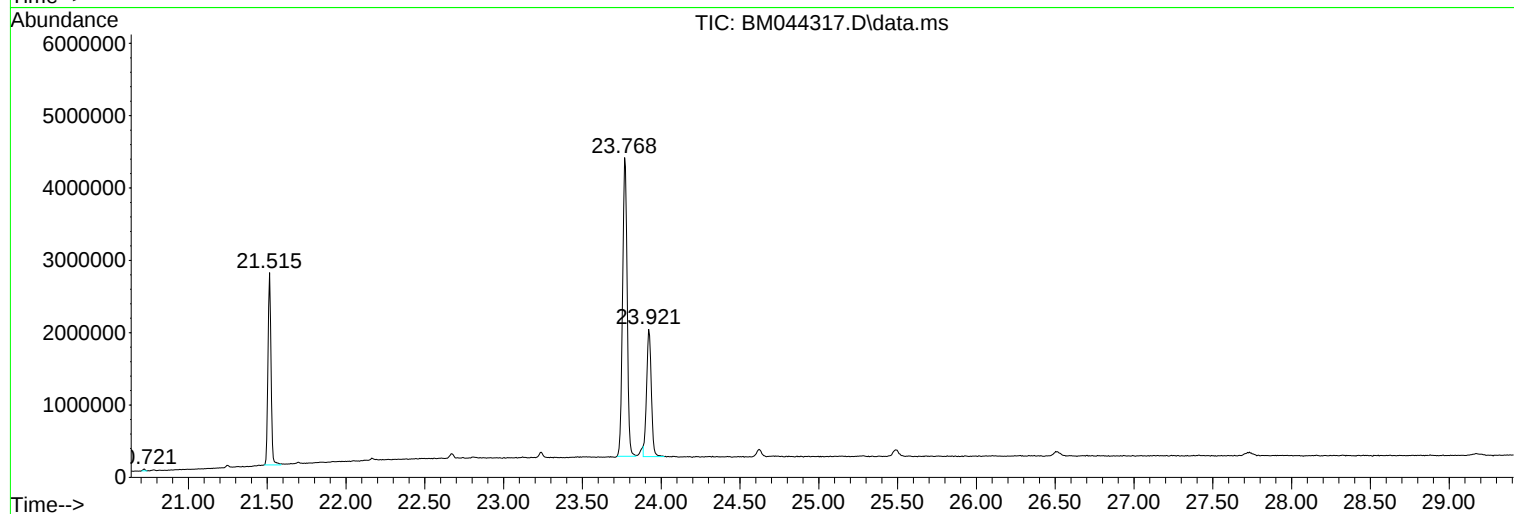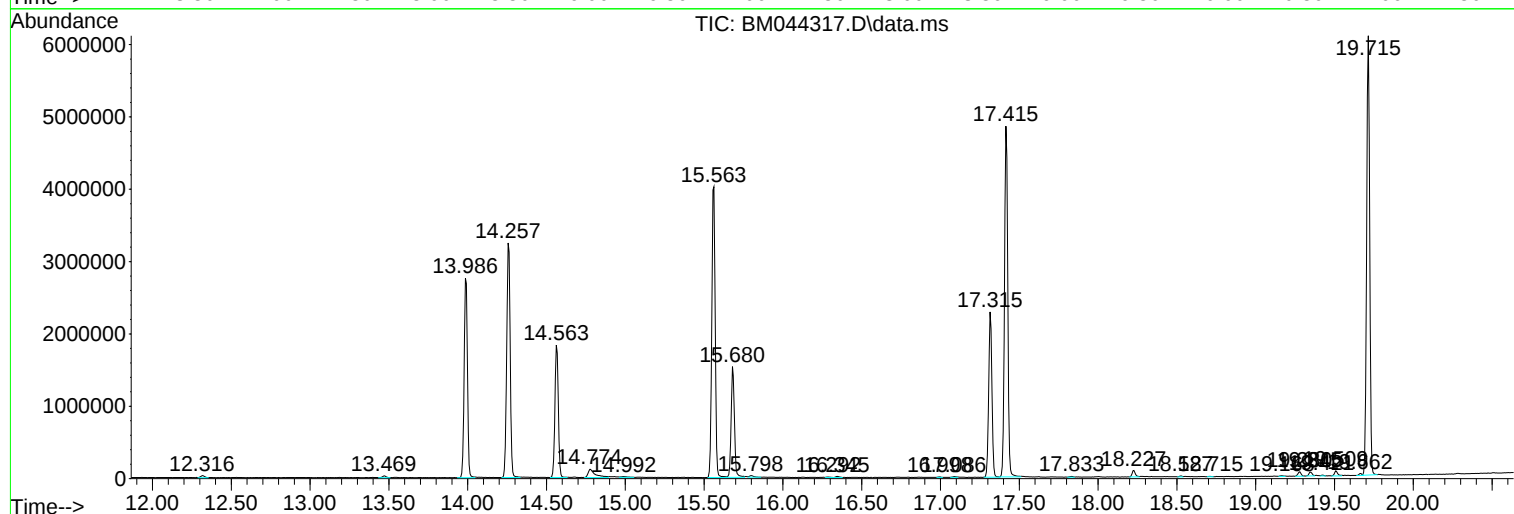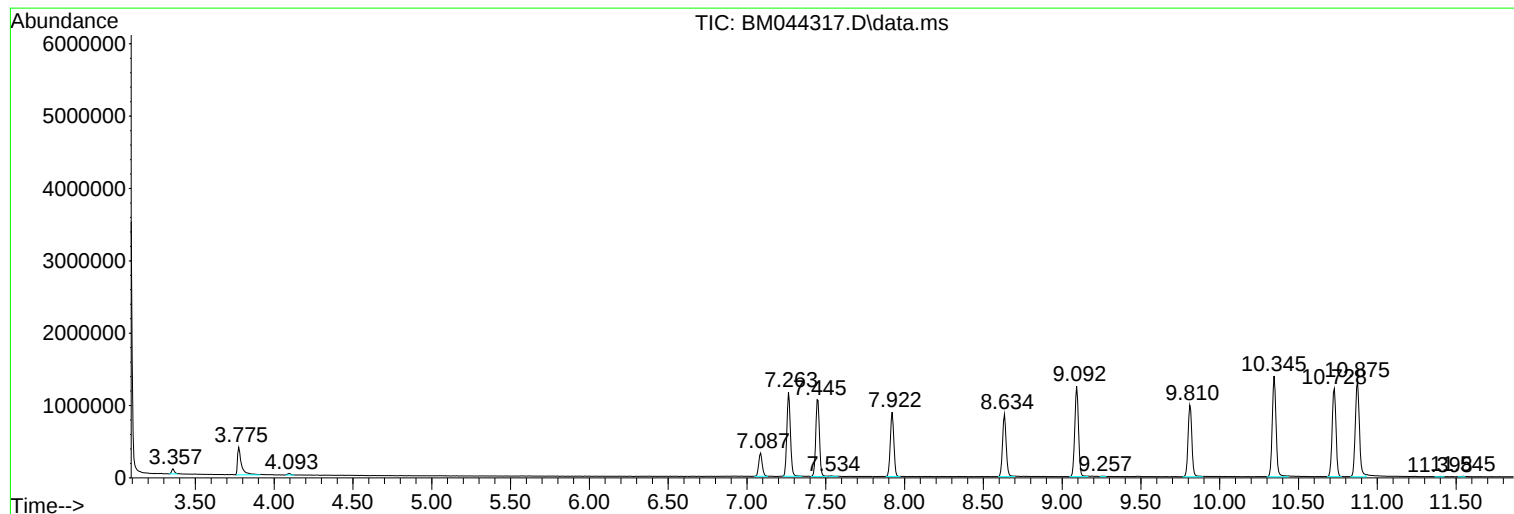

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044317.D
Acq On : 25 Feb 2024 04:59
Operator : MA/JU
Sample : P1494-08
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH410

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044317.D
Acq On : 25 Feb 2024 04:59
Operator : MA/JU
Sample : P1494-08
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH410

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------