

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
 Data File : BM044320.D
 Acq On : 25 Feb 2024 06:48
 Operator : MA/JU
 Sample : P1494-11
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3W1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044320.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.322	37	40	43	rBV	37908	43648	0.63%	0.078%
2	3.357	43	46	52	rVB	51479	64408	0.93%	0.115%
3	3.781	114	118	131	rBV	182607	328723	4.75%	0.589%
4	4.093	168	171	176	rVB2	13445	18626	0.27%	0.033%
5	7.087	674	680	691	rVB	210841	341581	4.94%	0.612%
6	7.263	703	710	722	rBV	890203	1417074	20.49%	2.538%
7	7.445	734	741	752	rBV	774233	1264085	18.28%	2.264%
8	7.534	754	756	762	rVB5	5770	7650	0.11%	0.014%
9	7.922	815	822	829	rBV	678985	1074802	15.54%	1.925%
10	8.634	935	943	953	rBV	582159	952647	13.77%	1.706%
11	9.092	1013	1021	1029	rBV	942855	1545763	22.35%	2.768%
12	9.257	1044	1049	1055	rVB8	11865	20699	0.30%	0.037%
13	9.481	1081	1087	1092	rVB4	5986	10593	0.15%	0.019%
14	9.810	1133	1143	1155	rBV	717809	1198642	17.33%	2.147%
15	10.345	1226	1234	1247	rBV	994685	1694511	24.50%	3.035%
16	10.728	1291	1299	1307	rBV	907622	1543910	22.32%	2.765%
17	10.875	1316	1324	1345	rBV	908402	1683134	24.33%	3.014%
18	12.316	1563	1569	1576	rBV	18348	34858	0.50%	0.062%
19	13.398	1749	1753	1757	rVB5	5263	7634	0.11%	0.014%
20	13.469	1757	1765	1770	rBV2	22311	37010	0.54%	0.066%
21	13.986	1847	1853	1865	rBV	2069339	2959041	42.78%	5.300%
22	14.257	1892	1899	1909	rBV	2356664	3567547	51.58%	6.389%
23	14.563	1945	1951	1964	rBV	1373912	1977606	28.59%	3.542%
24	14.786	1981	1989	2003	rBV	64518	217455	3.14%	0.389%
25	15.557	2113	2120	2132	rBV	3144509	4607955	66.62%	8.253%
26	15.680	2135	2141	2156	rVV	1155954	1648061	23.83%	2.952%
27	15.798	2157	2161	2169	rVB5	16681	33777	0.49%	0.060%
28	16.351	2251	2255	2261	rVB7	10465	17507	0.25%	0.031%
29	17.315	2412	2419	2429	rBV	1703524	2383871	34.47%	4.270%
30	17.415	2429	2436	2453	rVV	3990510	5685841	82.20%	10.183%
31	17.609	2467	2469	2474	rVB3	6337	9213	0.13%	0.017%
32	18.227	2568	2574	2581	rBV	86338	131918	1.91%	0.236%
33	19.274	2748	2752	2759	rVB	45386	66488	0.96%	0.119%
34	19.351	2760	2765	2770	rBV	43313	63577	0.92%	0.114%
35	19.427	2775	2778	2783	rVB6	9121	13083	0.19%	0.023%
36	19.509	2788	2792	2800	rBV2	48070	66064	0.96%	0.118%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044320.D
Acq On : 25 Feb 2024 06:48
Operator : MA/JU
Sample : P1494-11
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3W1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37	19.662	2815	2818	2820	rBV3	18169	21312	0.31%	0.038%
38	19.715	2820	2827	2837	rVB	4952141	6706999	96.97%	12.012%
39	20.715	2995	2997	3001	rBV4	15060	16735	0.24%	0.030%
40	21.245	3084	3087	3094	rBV7	43793	64002	0.93%	0.115%
41	21.515	3128	3133	3143	rBV	2018134	2576016	37.24%	4.614%
42	23.768	3508	3516	3529	rBV2	3423191	6916723	100.00%	12.388%
43	23.921	3536	3542	3555	rVB	1314735	2793848	40.39%	5.004%




Sum of corrected areas: 55834637

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044320.D
Acq On : 25 Feb 2024 06:48
Operator : MA/JU
Sample : P1494-11
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3W1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

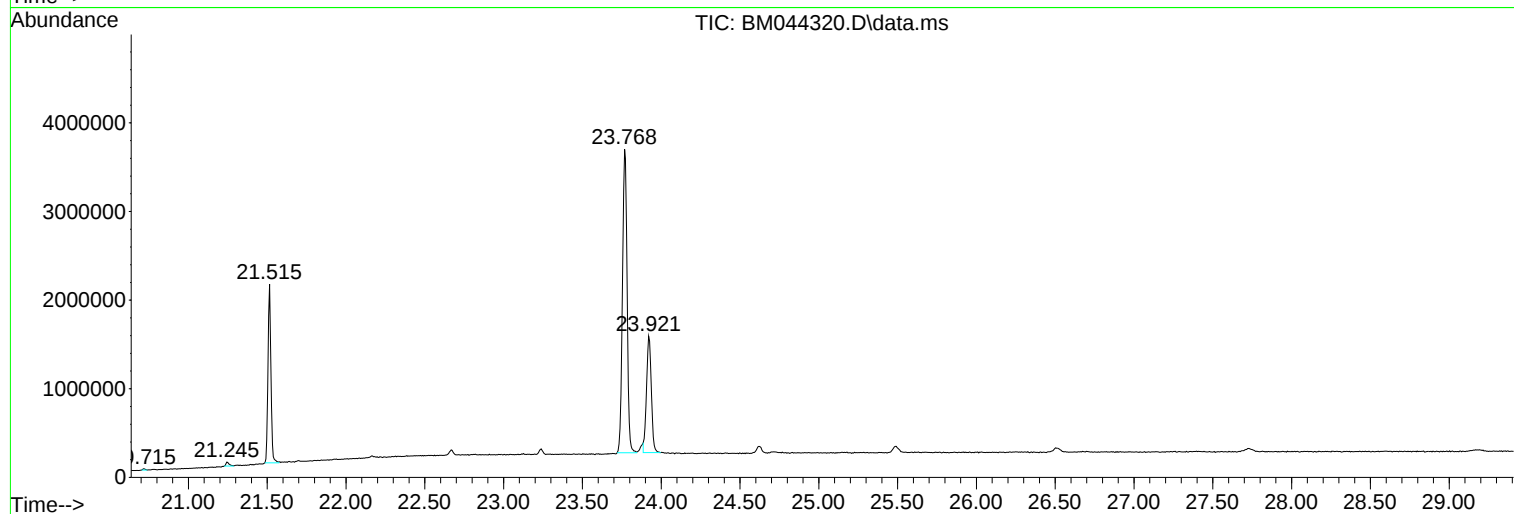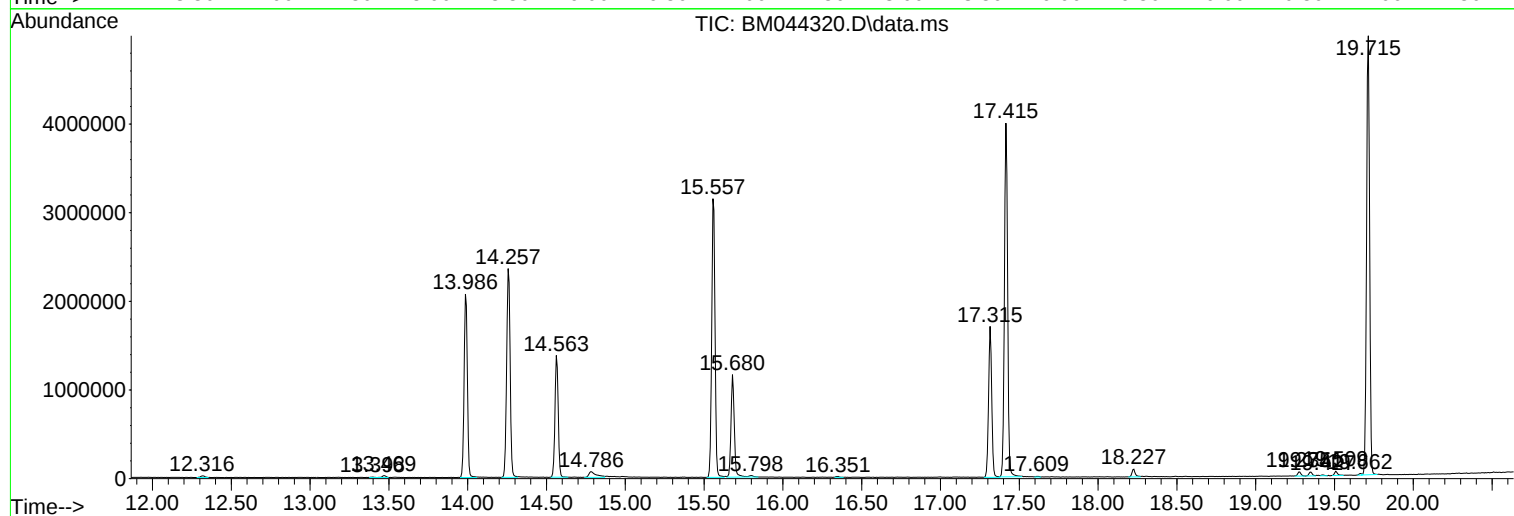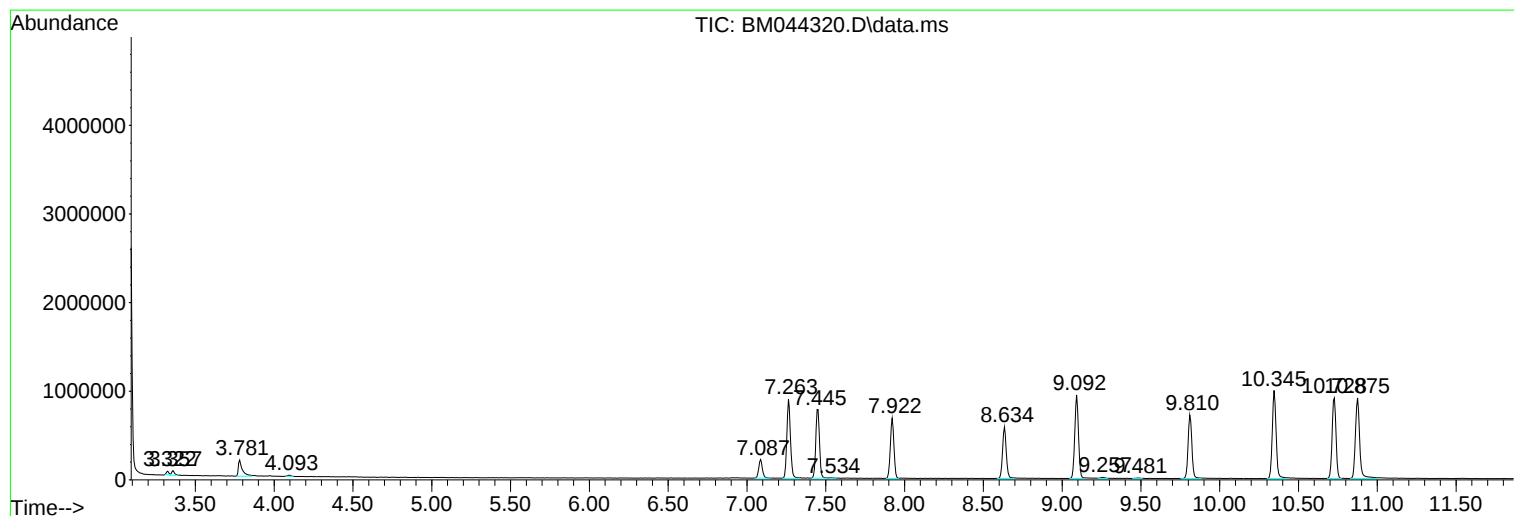

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044320.D
Acq On : 25 Feb 2024 06:48
Operator : MA/JU
Sample : P1494-11
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3W1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044320.D
Acq On : 25 Feb 2024 06:48
Operator : MA/JU
Sample : P1494-11
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3W1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------