

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
 Data File : BM044321.D
 Acq On : 25 Feb 2024 07:24
 Operator : MA/JU
 Sample : P1494-12
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3W2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044321.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.357	42	46	53	rVB	55583	72001	1.04%	0.127%
2	3.781	114	118	132	rBV	191245	348239	5.01%	0.612%
3	4.093	168	171	175	rVB	17662	22012	0.32%	0.039%
4	7.087	674	680	692	rVB	227809	365443	5.26%	0.642%
5	7.263	702	710	725	rBV	937081	1496400	21.54%	2.629%
6	7.445	735	741	750	rBV	832330	1346077	19.38%	2.365%
7	7.922	814	822	829	rBV	692831	1077078	15.51%	1.892%
8	8.634	936	943	957	rBV	623193	1016995	14.64%	1.787%
9	9.092	1014	1021	1033	rBV	979618	1639004	23.60%	2.880%
10	9.192	1035	1038	1044	rVV6	7911	14483	0.21%	0.025%
11	9.257	1046	1049	1055	rVB8	7717	11751	0.17%	0.021%
12	9.481	1083	1087	1093	rVB8	4714	7951	0.11%	0.014%
13	9.810	1135	1143	1154	rBV	741837	1251047	18.01%	2.198%
14	10.086	1187	1190	1196	rVB8	3473	7130	0.10%	0.013%
15	10.345	1227	1234	1250	rBV	1035742	1760235	25.34%	3.093%
16	10.728	1291	1299	1306	rBV	917669	1557279	22.42%	2.736%
17	10.875	1314	1324	1345	rBV	891224	1685908	24.27%	2.962%
18	12.322	1564	1570	1577	rVB2	21986	37712	0.54%	0.066%
19	12.927	1668	1673	1677	rBV6	5017	7747	0.11%	0.014%
20	13.192	1712	1718	1724	rBV	17767	28101	0.40%	0.049%
21	13.469	1760	1765	1774	rBV3	17583	32435	0.47%	0.057%
22	13.539	1774	1777	1785	rVB7	4745	8126	0.12%	0.014%
23	13.986	1846	1853	1864	rBV	2088253	3051161	43.92%	5.361%
24	14.257	1891	1899	1912	rBV	2446619	3702611	53.30%	6.505%
25	14.563	1942	1951	1960	rBV	1334223	1996001	28.73%	3.507%
26	14.786	1981	1989	2003	rBV3	69640	233061	3.36%	0.409%
27	14.980	2020	2022	2030	rVB8	6743	12423	0.18%	0.022%
28	15.368	2083	2088	2094	rBV	41256	54398	0.78%	0.096%
29	15.563	2113	2121	2135	rBV	3221550	4738349	68.21%	8.325%
30	15.680	2135	2141	2154	rVV	1145666	1647972	23.72%	2.895%
31	15.798	2157	2161	2166	rVB5	16241	29305	0.42%	0.051%
32	16.345	2251	2254	2258	rVB6	11610	16030	0.23%	0.028%
33	16.733	2315	2320	2322	rBV6	5327	7383	0.11%	0.013%
34	17.315	2412	2419	2430	rBV	1681799	2397932	34.52%	4.213%
35	17.415	2430	2436	2457	rVV2	3969068	5787622	83.32%	10.169%
36	18.227	2569	2574	2581	rBV	56408	86443	1.24%	0.152%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
 Data File : BM044321.D
 Acq On : 25 Feb 2024 07:24
 Operator : MA/JU
 Sample : P1494-12
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3W2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

37	19.280	2748	2753	2758	rBV	47267	64310	0.93%	0.113%
38	19.351	2758	2765	2769	rBV	43207	64358	0.93%	0.113%
39	19.392	2769	2772	2776	rVV6	10001	16496	0.24%	0.029%
40	19.427	2776	2778	2782	rVB5	7079	8044	0.12%	0.014%
41	19.509	2788	2792	2799	rBV3	40360	62315	0.90%	0.109%
42	19.662	2815	2818	2821	rBV3	23483	26078	0.38%	0.046%
43	19.715	2821	2827	2836	rVV	5129777	6745836	97.11%	11.852%
44	19.974	2867	2871	2876	rVB2	59987	69647	1.00%	0.122%
45	20.721	2995	2998	3002	rVB4	15792	15659	0.23%	0.028%
46	21.515	3127	3133	3148	rBV	1944585	2642415	38.04%	4.643%
47	23.768	3508	3516	3530	rBV2	3515304	6946338	100.00%	12.204%
48	23.921	3536	3542	3551	rVB	1328511	2701569	38.89%	4.747%




Sum of corrected areas: 56916910

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044321.D
Acq On : 25 Feb 2024 07:24
Operator : MA/JU
Sample : P1494-12
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3W2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

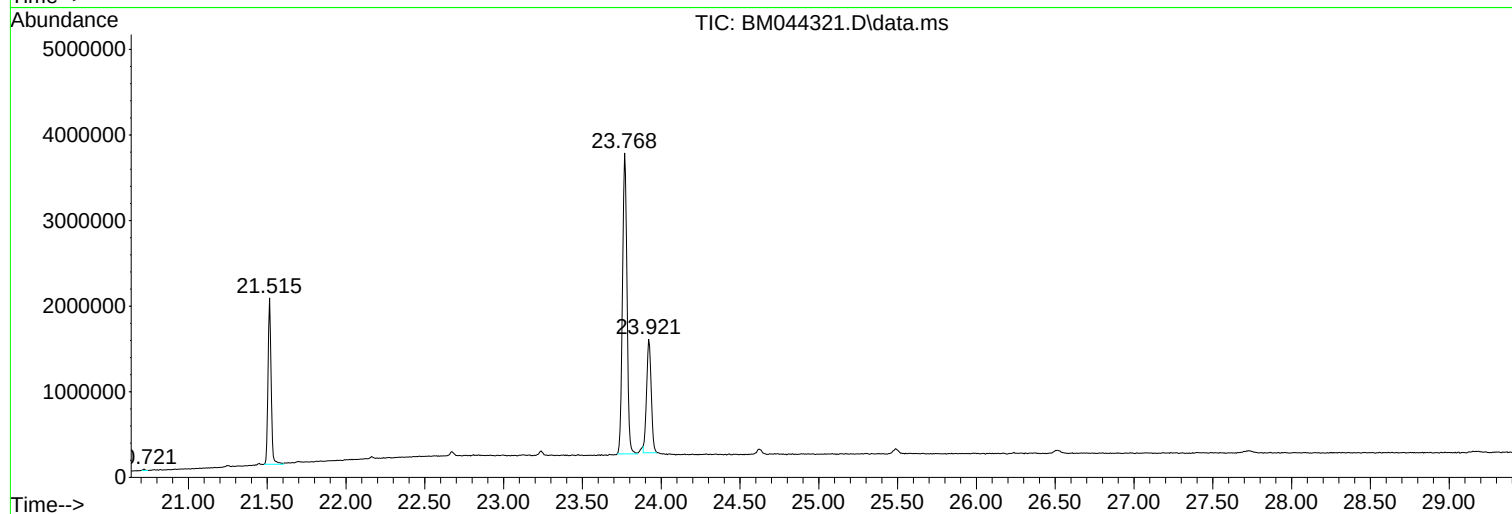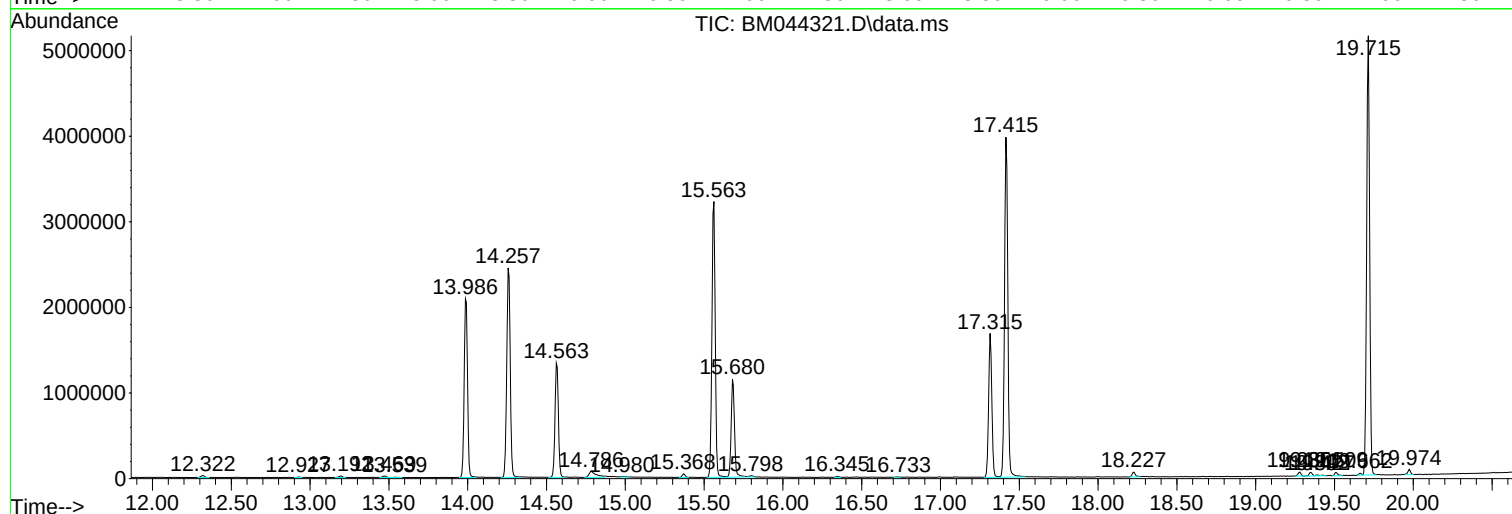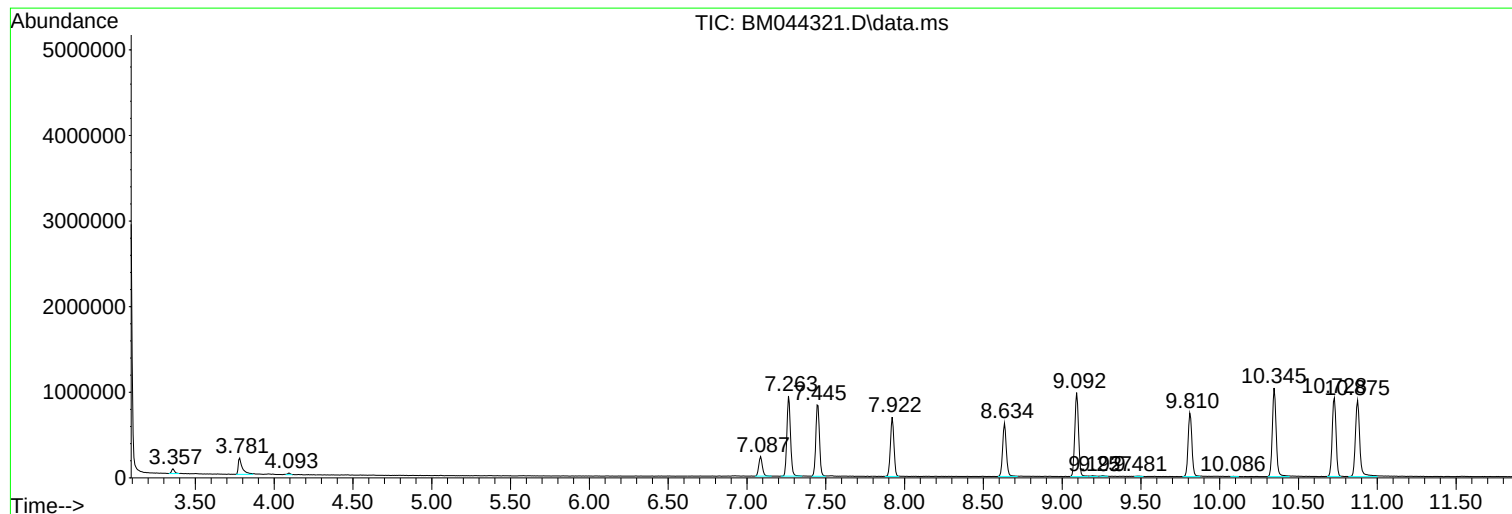

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044321.D
Acq On : 25 Feb 2024 07:24
Operator : MA/JU
Sample : P1494-12
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3W2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022424\
Data File : BM044321.D
Acq On : 25 Feb 2024 07:24
Operator : MA/JU
Sample : P1494-12
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3W2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------