

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022516\
 Data File : BM004401.D
 Acq On : 25 Feb 2016 14:42
 Operator : SJ/UM
 Sample : PB88515BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK15

Quant Time: Feb 26 01:32:29 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 26 01:28:38 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	22452	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	106853	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.28	164	66453	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	145915	20.00	ng/ul	0.00
78) Chrysene-d12	21.25	240	132357	20.00	ng/ul	0.00
86) Perylene-d12	23.48	264	121779	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.08	96	2106	4.94	ng/uL	0.00
5) Phenol-d5	6.80	99	43331	23.02	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	24054	25.12	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	40279	24.81	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	40226	23.91	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	20785	25.57	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	24261	26.18	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	39418	23.53	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	61555	29.48	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	156790	27.51	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	178658	26.78	ng/ul	0.00
52) 4-Nitrophenol-d4	14.53	143	20243	22.10	ng/ul	0.00
58) Fluorene-d10	15.28	176	128784	26.57	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.43	200	16135	18.00	ng/ul	0.00
71) Anthracene-d10	17.13	188	200505	28.04	ng/ul	0.00
79) Pyrene-d10	19.44	212	204053	31.87	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.34	264	185690	29.06	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
76) Di-n-butylphthalate	18.00	149	12728	1.18	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022516\
Data File : BM004401.D
Acq On : 25 Feb 2016 14:42
Operator : SJ/UM
Sample : PB88515BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK15

Quant Time: Feb 26 01:32:29 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 26 01:28:38 2016
Response via : Initial Calibration

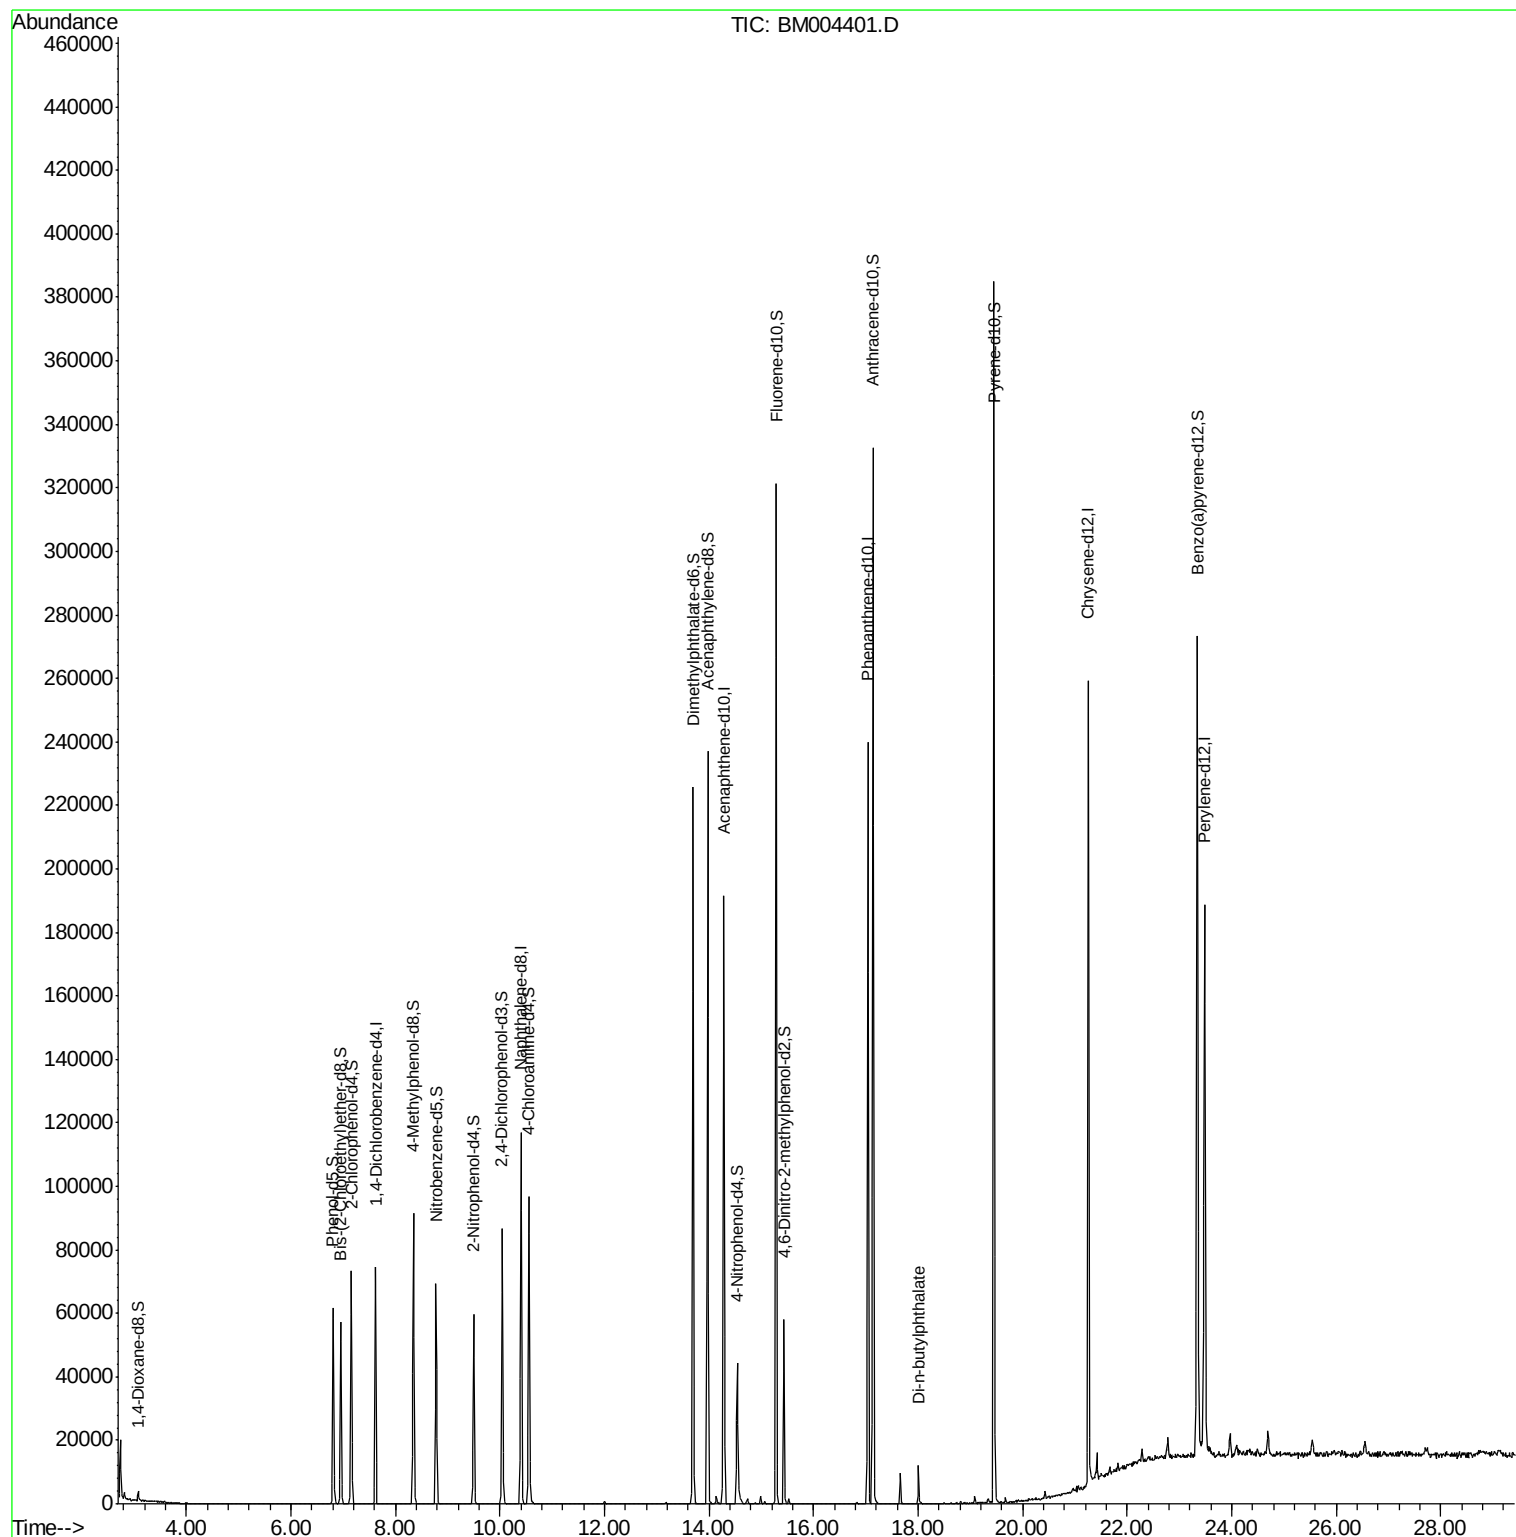

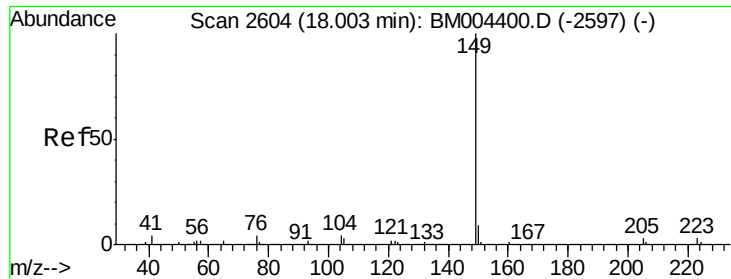

#76
 Di-n-butylphthalate
 Concen: 1.18 ng/ul
 RT: 18.00 min Scan# 2604
 Delta R.T. 0.00 min
 Lab File: BM004401.D
 Acq: 25 Feb 2016 14:42

Instrument :
 BNA_M
 ClientSampleId :
 SBLK15

Tgt Ion:149 Resp: 12728
 Ion Ratio Lower Upper
 149 100
 150 9.6 7.4 11.0
 104 4.4 4.0 6.0

