

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022516\
 Data File : BM004402.D
 Acq On : 25 Feb 2016 16:43
 Operator : SJ/UM
 Sample : PB88538BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK38

Quant Time: Feb 26 01:32:36 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 26 01:28:38 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	22115	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	100168	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.28	164	60928	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	132271	20.00	ng/ul	0.00
78) Chrysene-d12	21.26	240	134167	20.00	ng/ul	0.00
86) Perylene-d12	23.48	264	133892	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.07	96	2462	5.87	ng/uL	0.00
5) Phenol-d5	6.80	99	50403	27.18	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	27679	29.35	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	46250	28.92	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	46070	27.80	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	23812	31.25	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	27524	31.68	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	44395	28.27	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	70051	35.79	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	174550	33.40	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	199852	32.67	ng/ul	0.00
52) 4-Nitrophenol-d4	14.53	143	26389	31.42	ng/ul	0.00
58) Fluorene-d10	15.28	176	142487	32.06	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.43	200	21457	26.41	ng/ul	0.00
71) Anthracene-d10	17.13	188	236701	36.52	ng/ul	0.00
79) Pyrene-d10	19.45	212	249444	38.44	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.34	264	262641	37.38	ng/ul	0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
76) Di-n-butylphthalate	18.00	149	21391	2.19	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022516\
Data File : BM004402.D
Acq On : 25 Feb 2016 16:43
Operator : SJ/UM
Sample : PB88538BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK38

Quant Time: Feb 26 01:32:36 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 26 01:28:38 2016
Response via : Initial Calibration

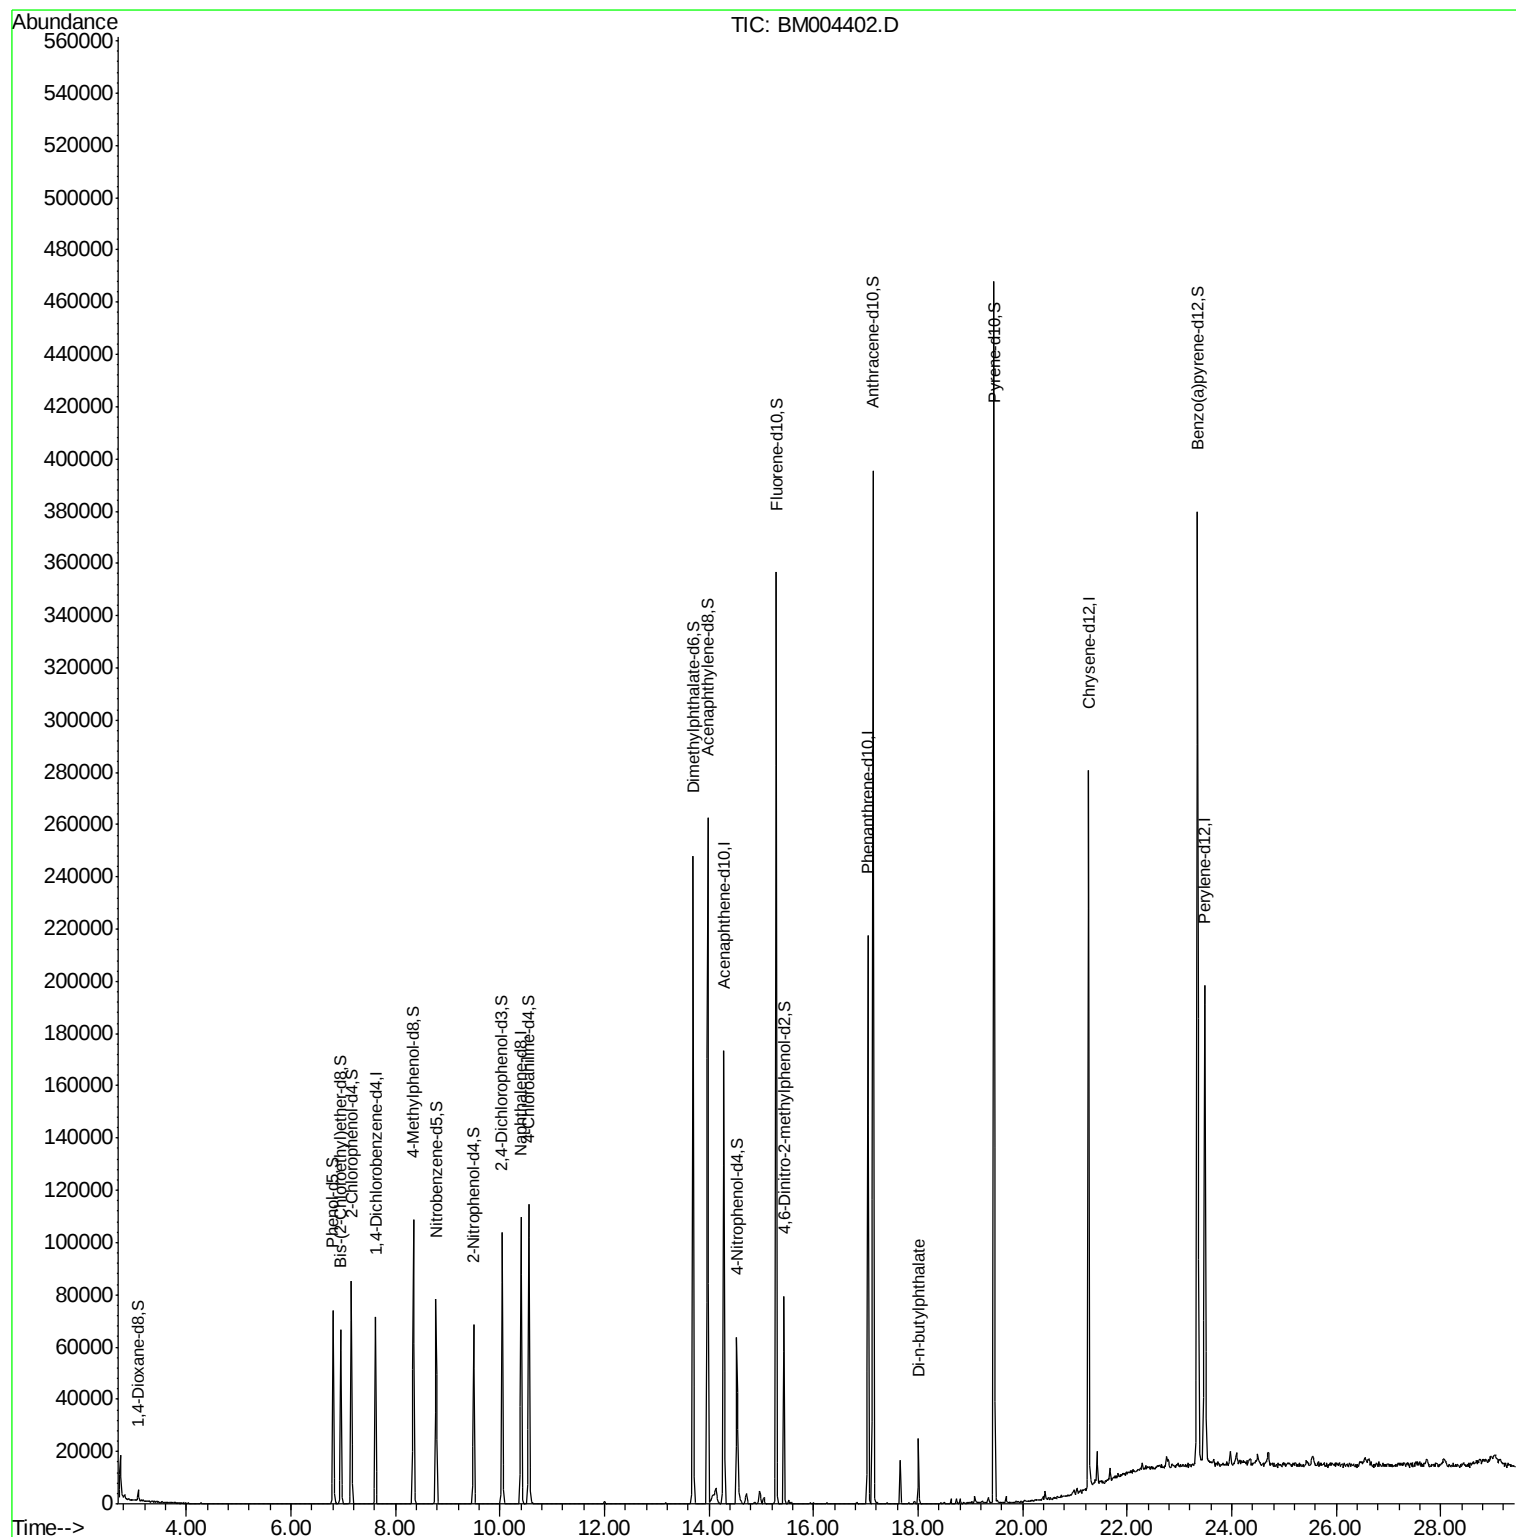

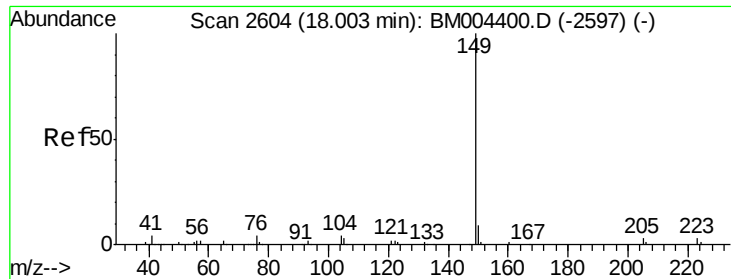

#76
 Di-n-butylphthalate
 Concen: 2.19 ng/ul
 RT: 18.00 min Scan# 2604
 Delta R.T. -0.00 min
 Lab File: BM004402.D
 Acq: 25 Feb 2016 16:43

Instrument :
 BNA_M
 ClientSampleId :
 SBLK38

Tgt Ion:149 Resp: 21391
 Ion Ratio Lower Upper
 149 100
 150 8.7 7.4 11.0
 104 4.4 4.0 6.0

